

Fig. 1a

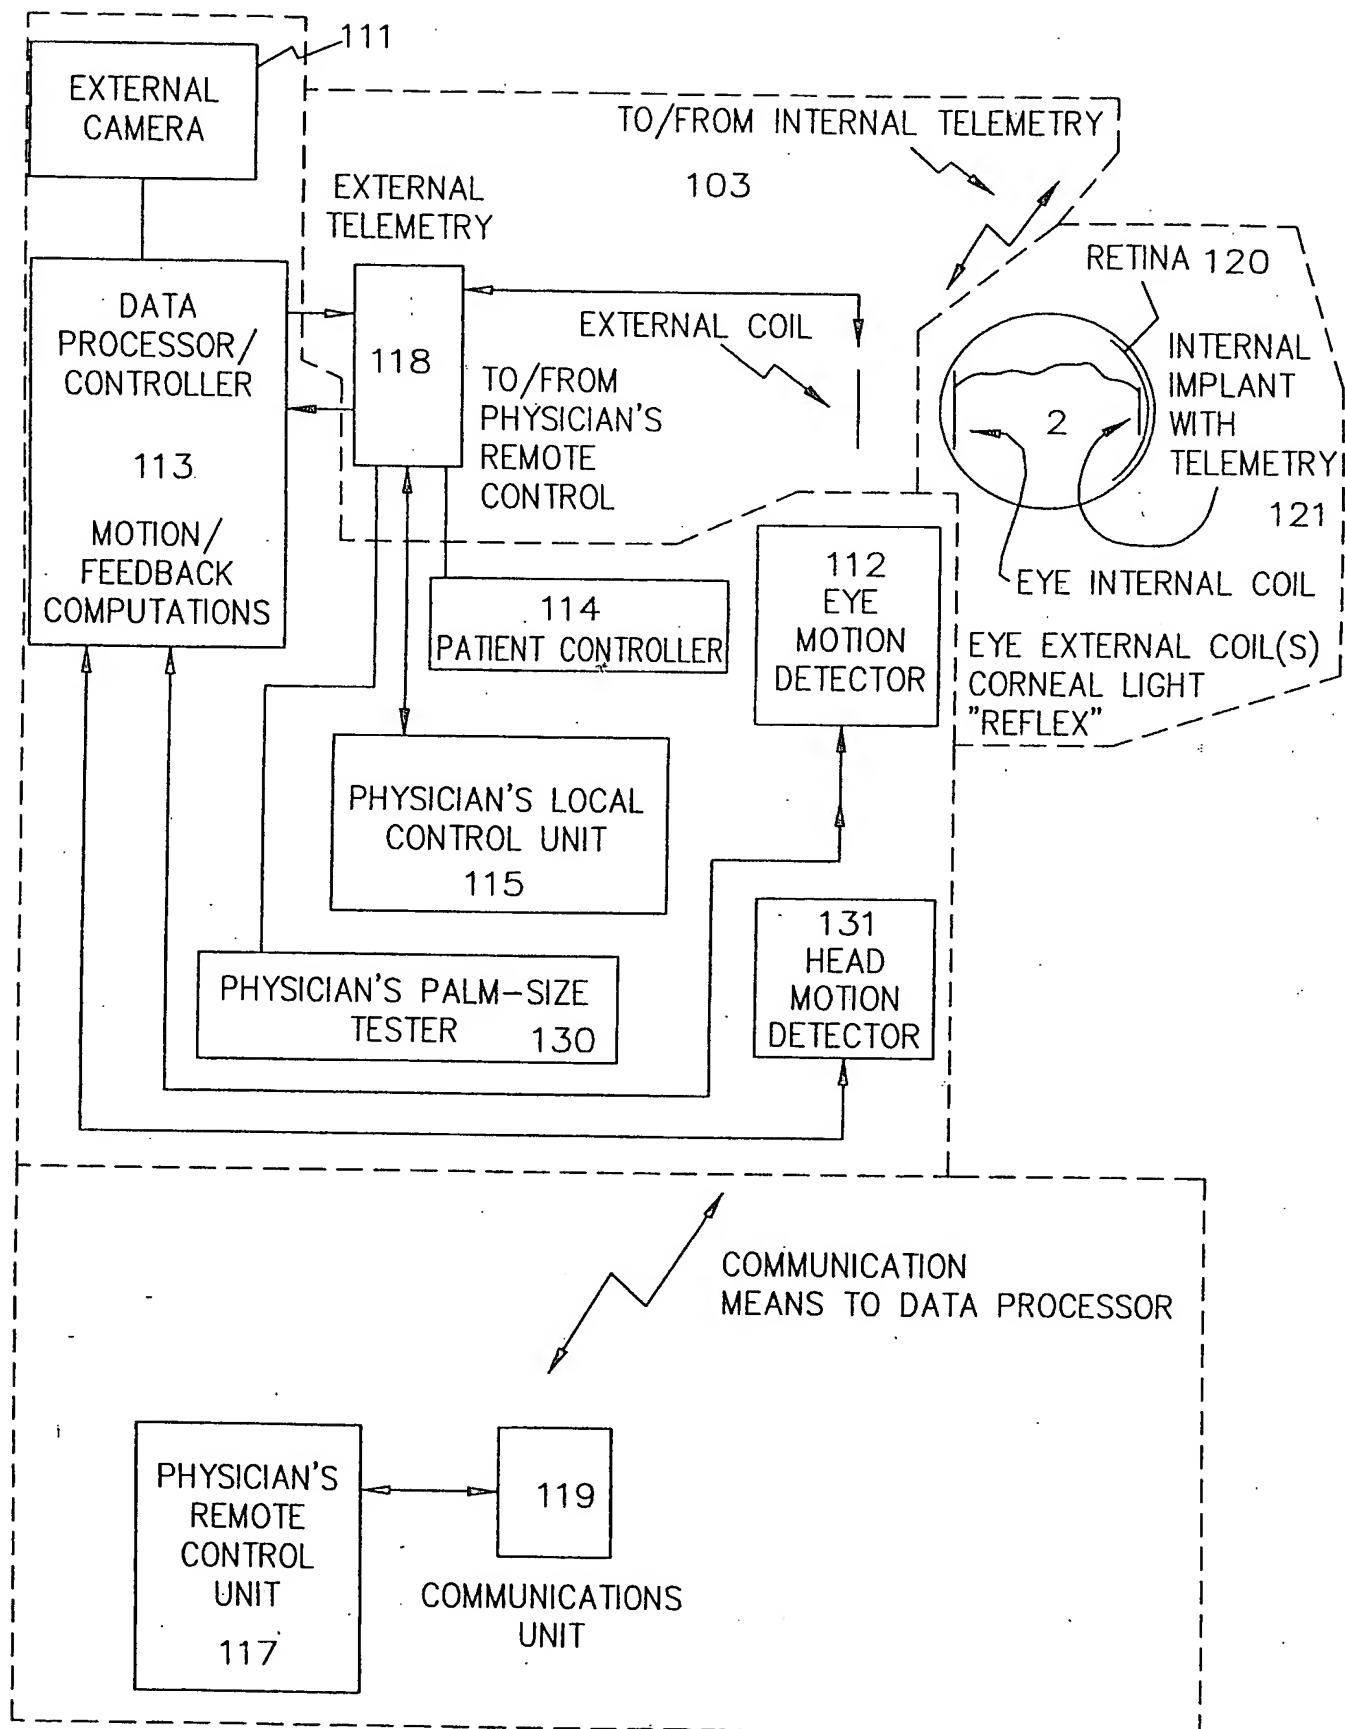


FIGURE 1b

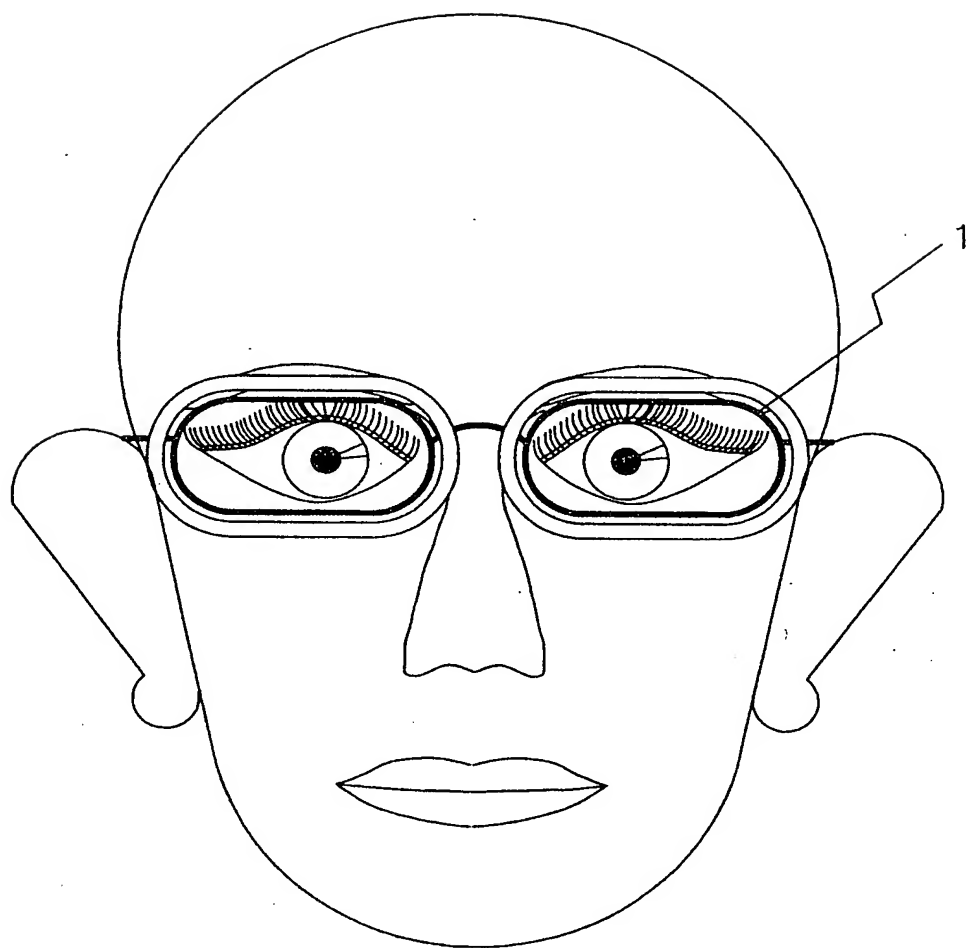


Fig. 1c

Patent 4,000,000

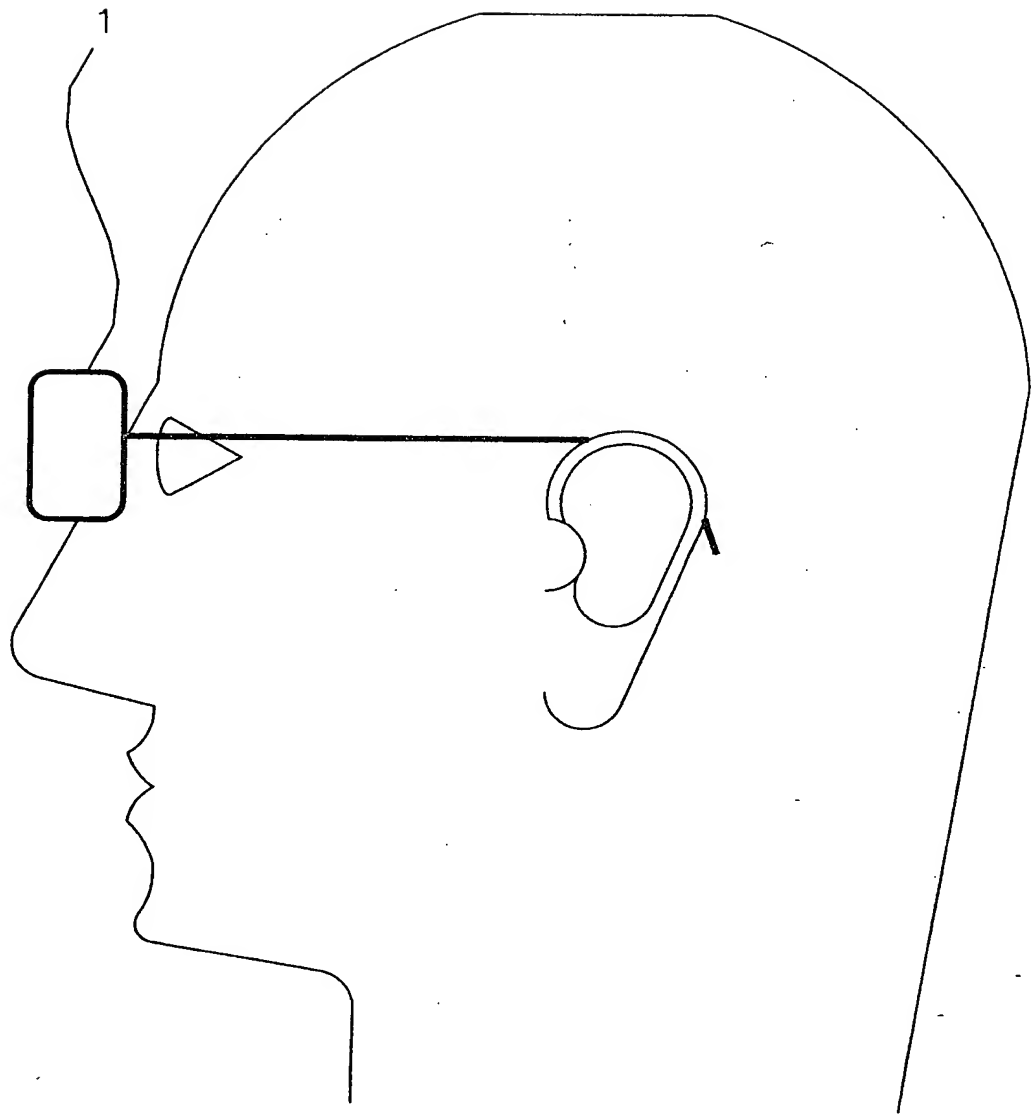


Fig 1d

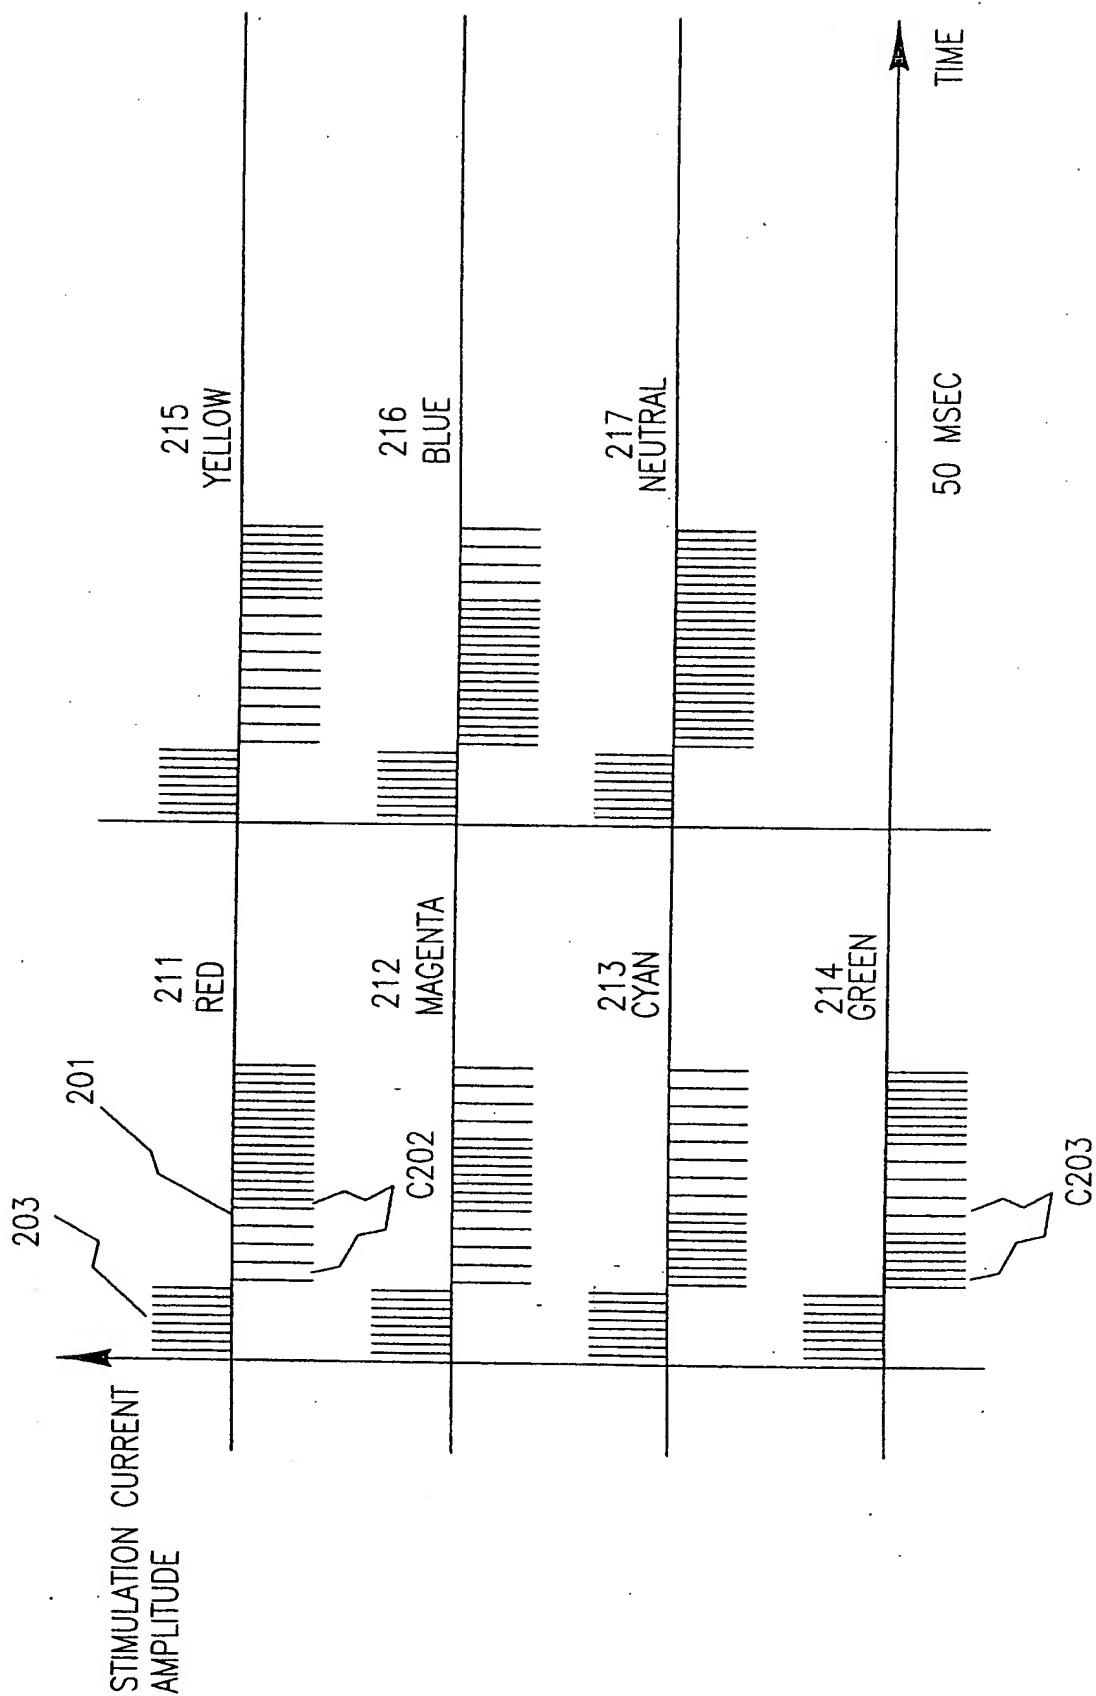


FIGURE 2a  
COLOR CODING

FIG. 2b

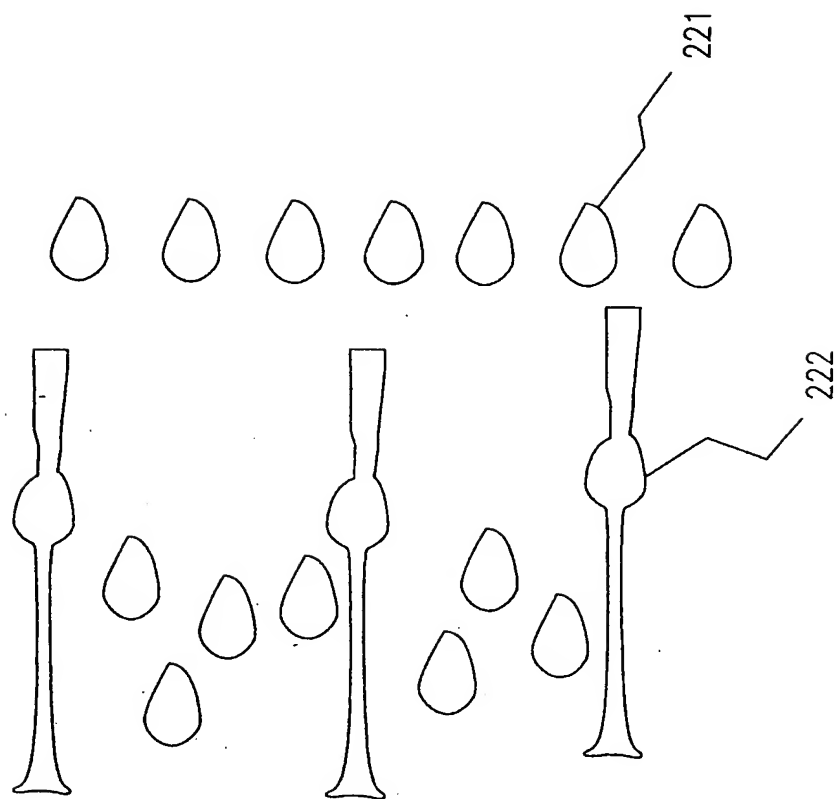


FIGURE 2b

FIG. 2c


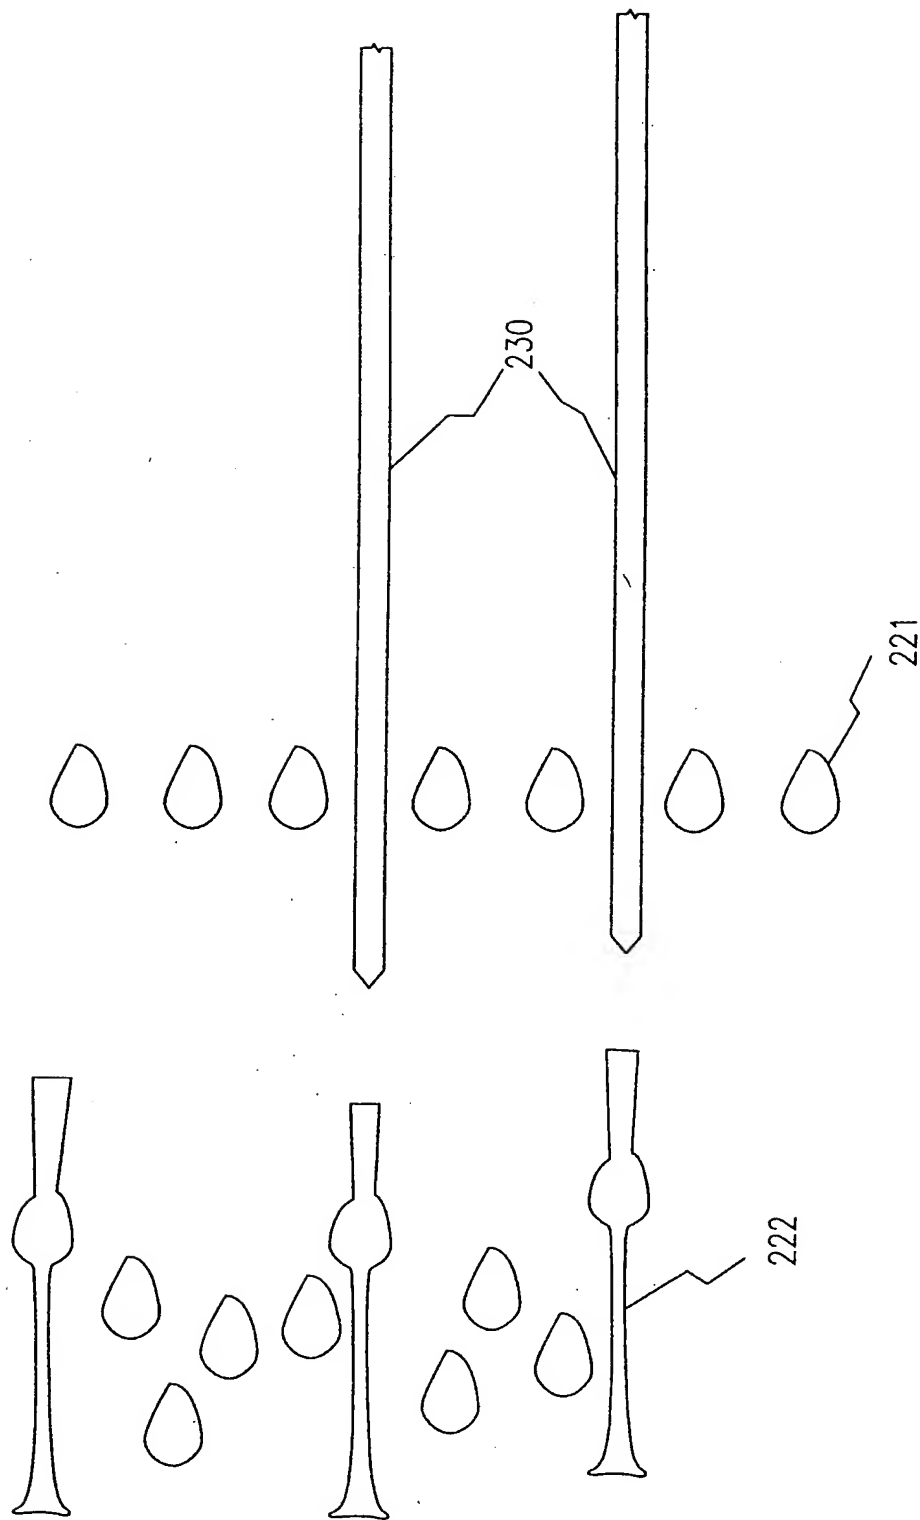


FIGURE 2c



EXTERNAL/INTERNAL TELEMETRY UNIT —  
EXTERNAL COIL/INTERNAL COIL /INTERNAL CHIP

FIGURE 3a

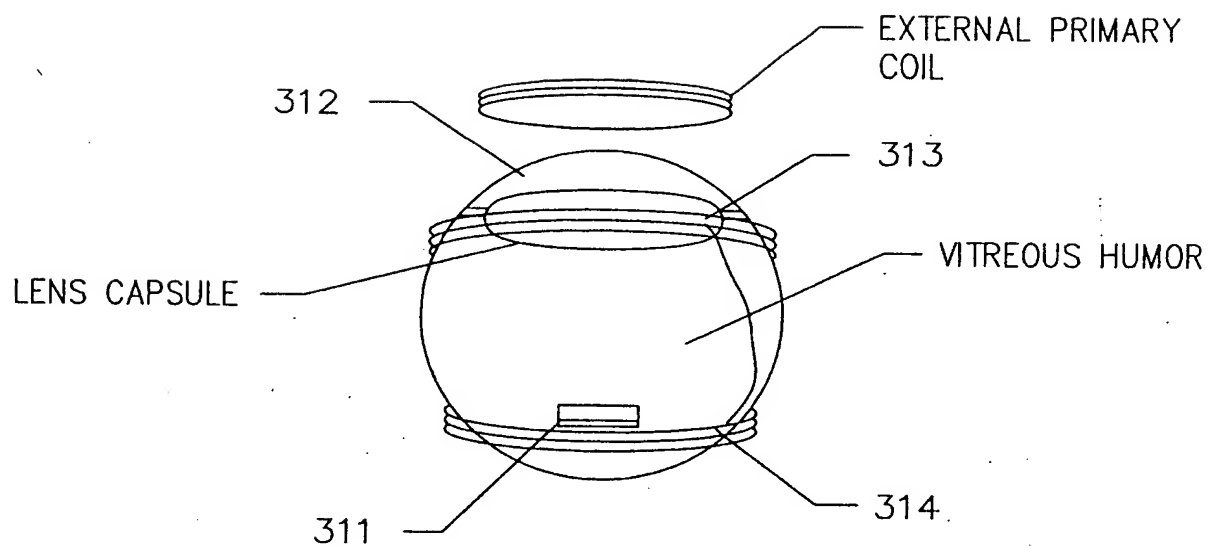

4039837 401801

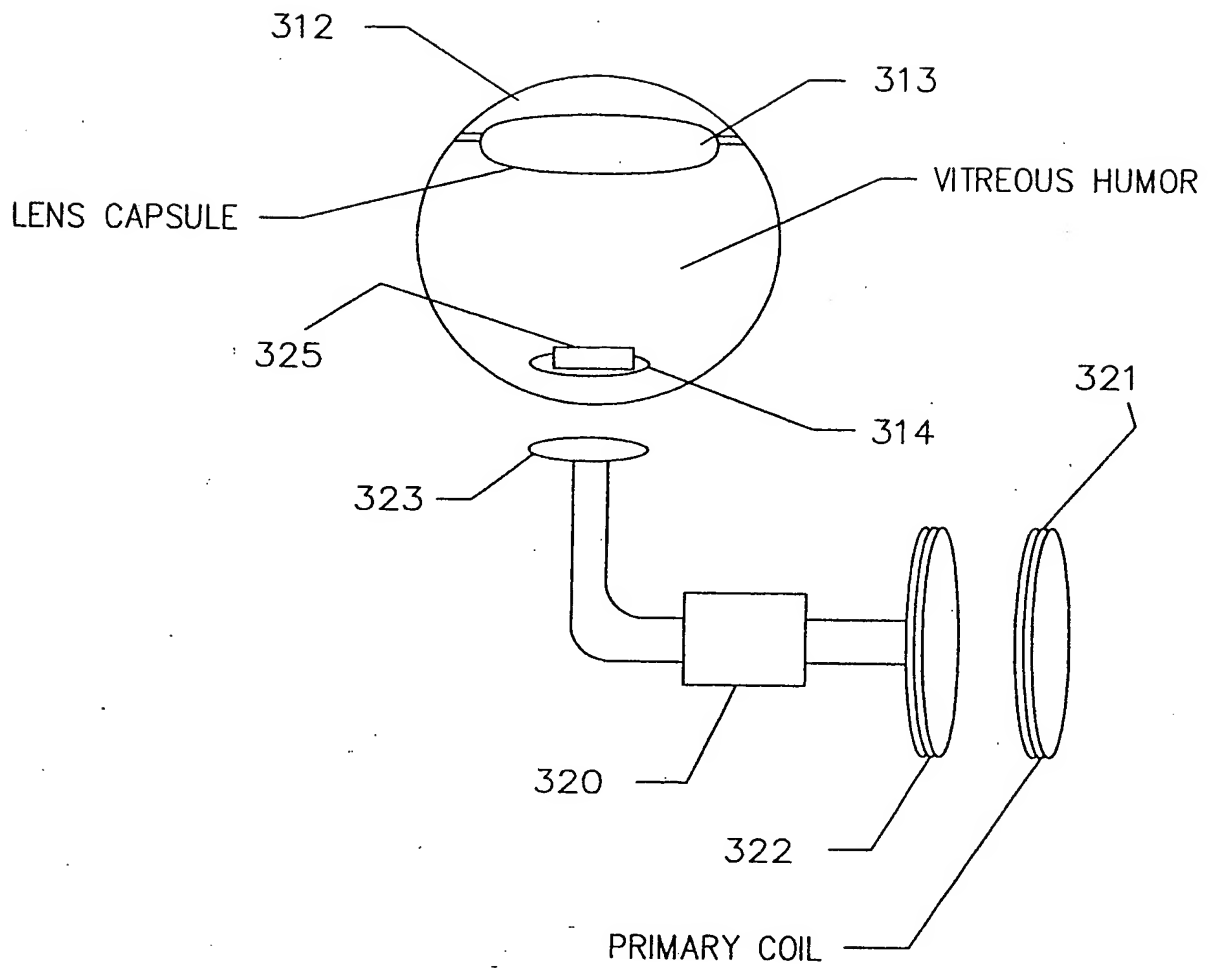


FIGURE 3b

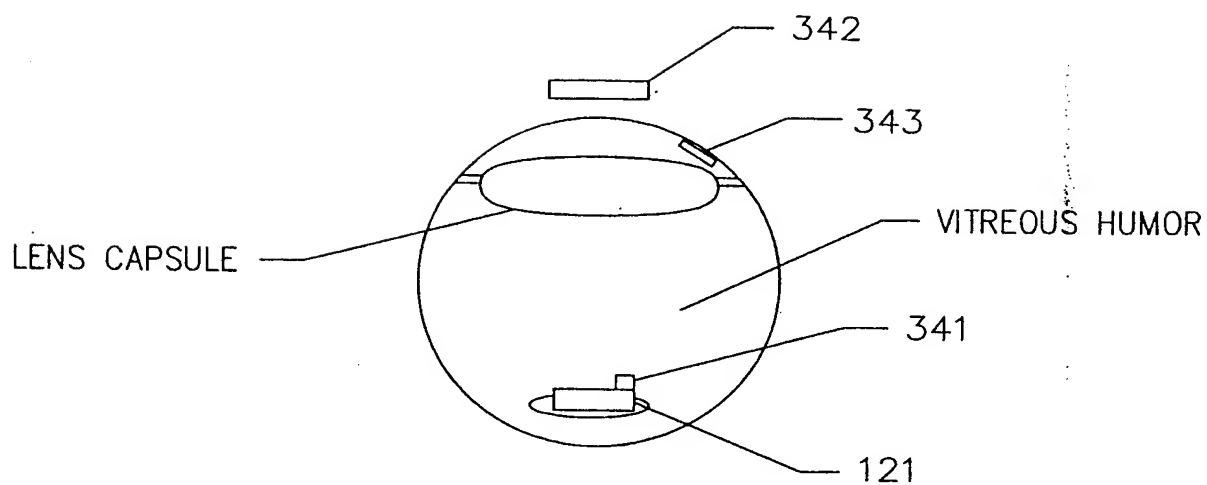


FIGURE 3c




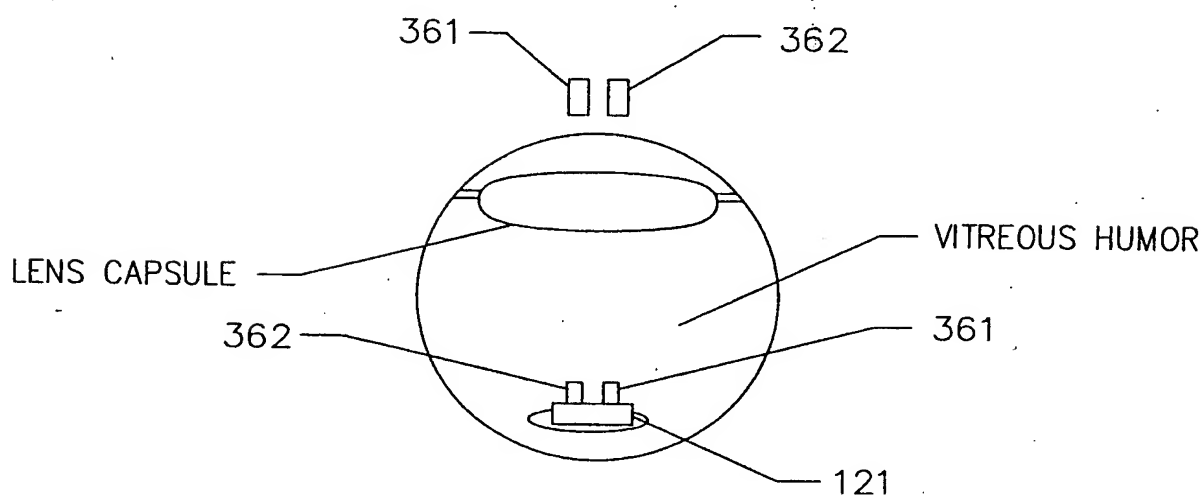


FIGURE 3d

4039837 401804

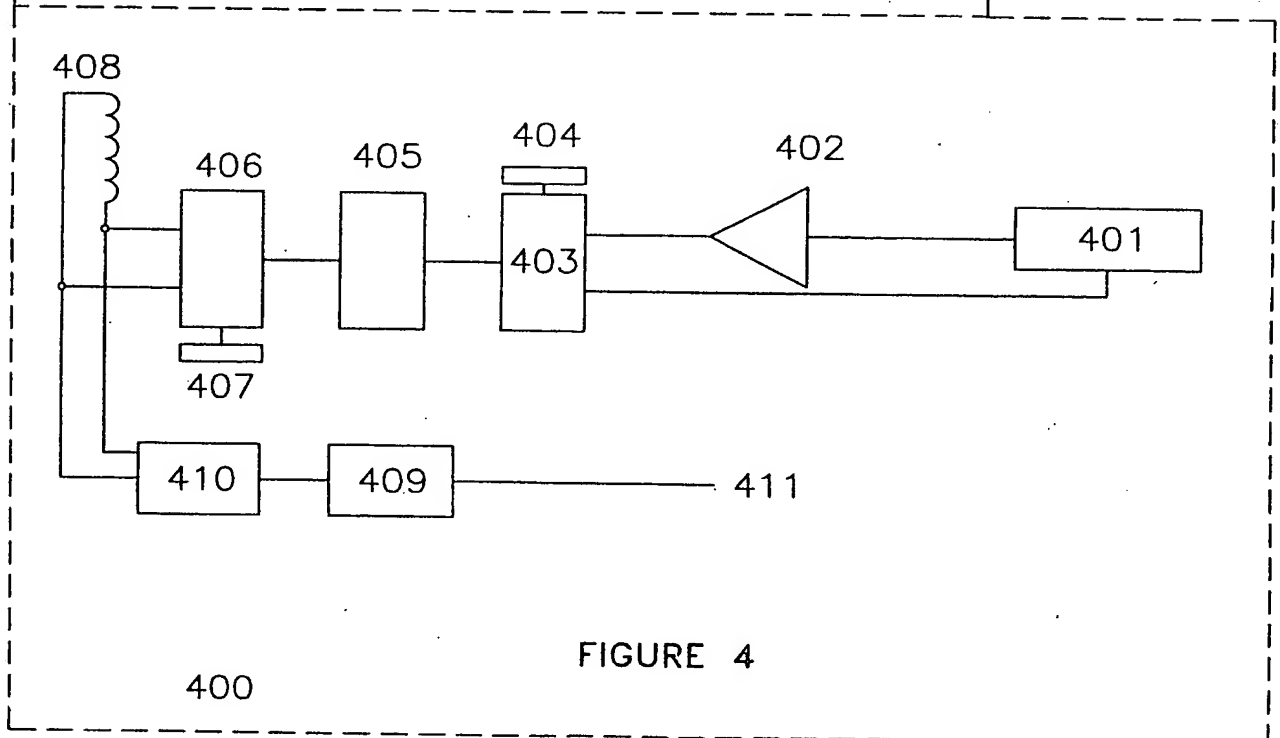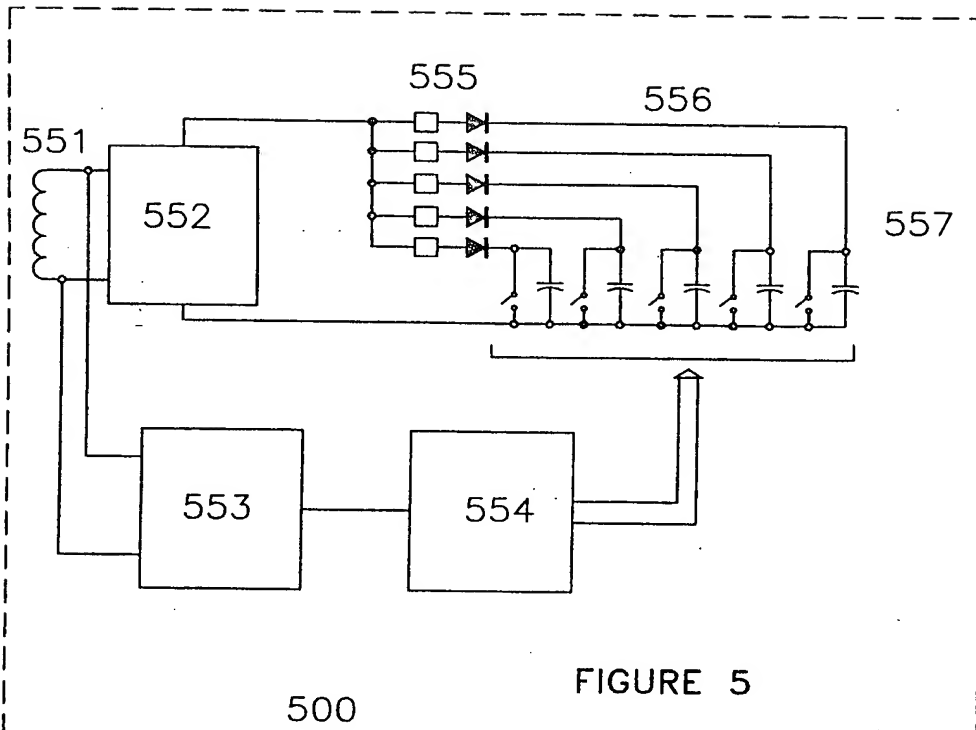

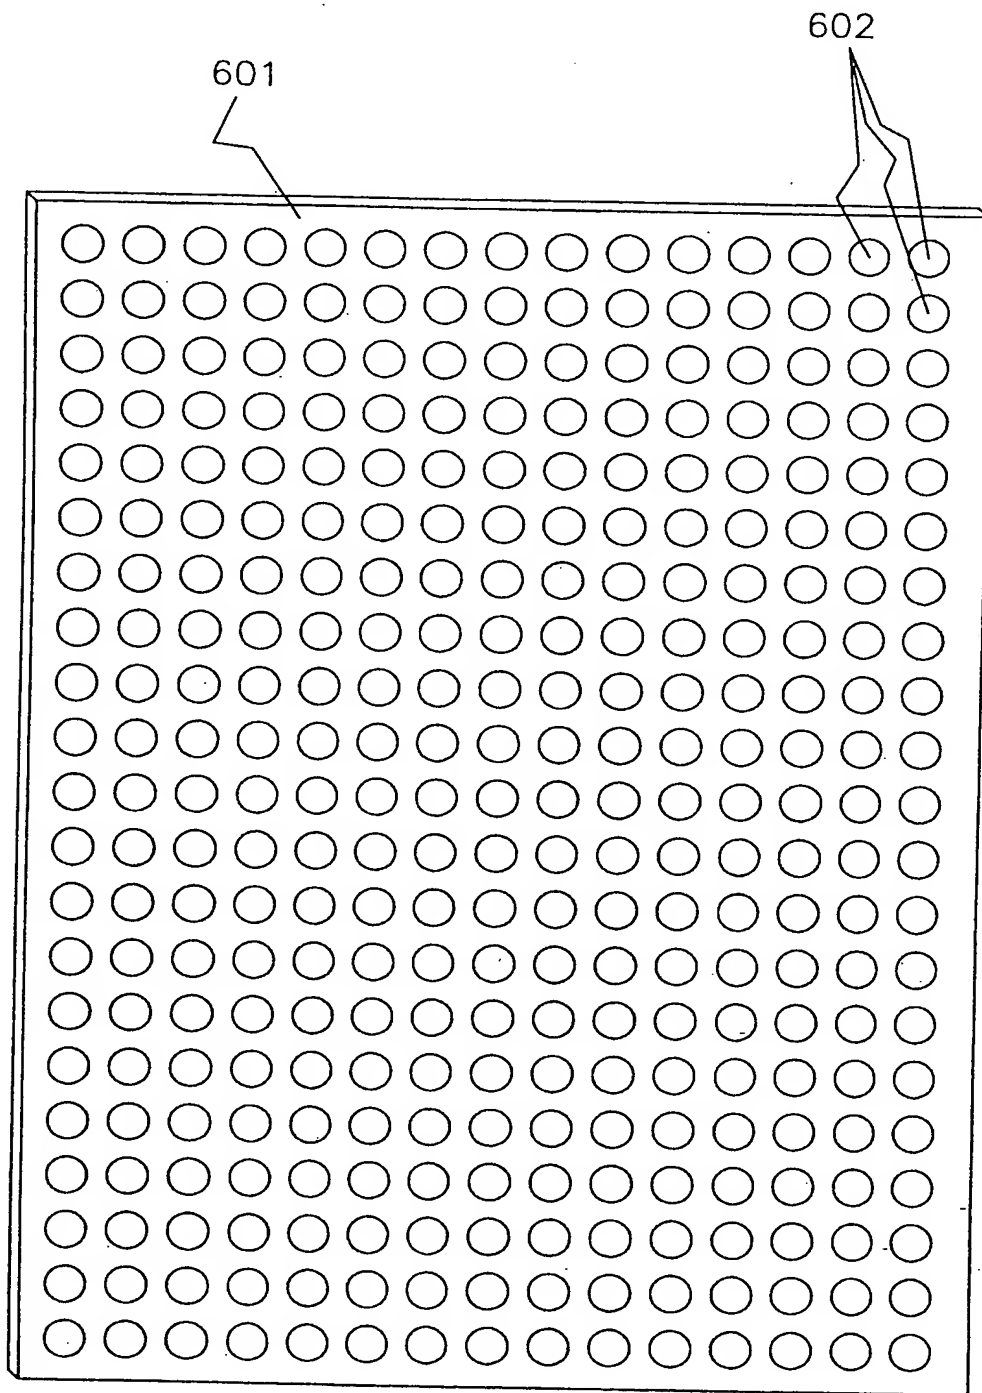

ELECTRODES ON SUBSTRATE

FIGURE 6a

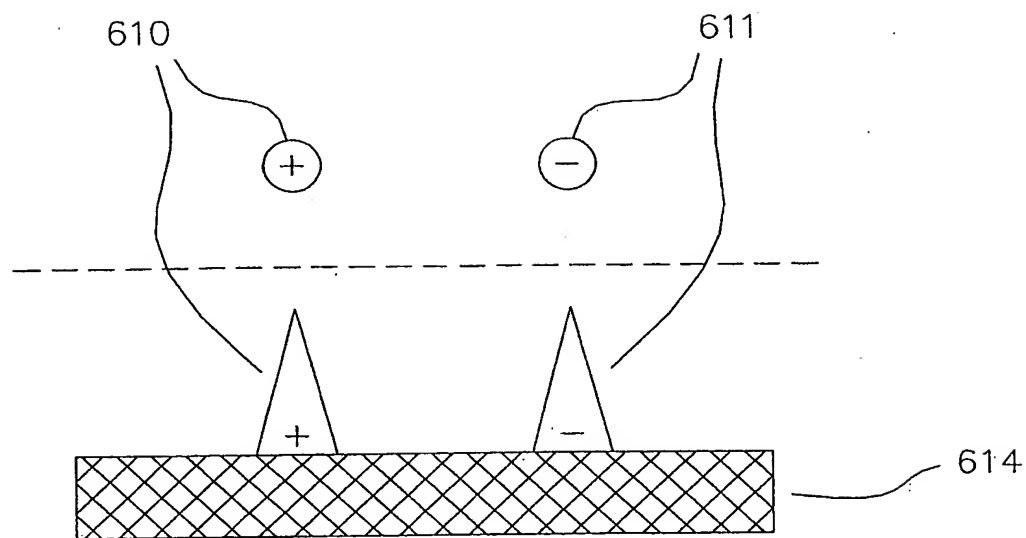


FIGURE 6b



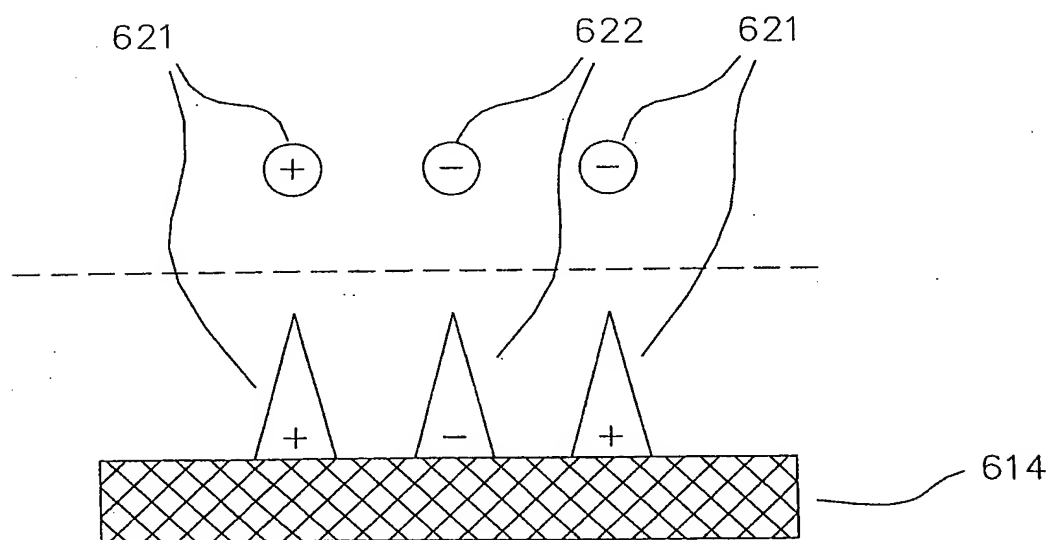



FIGURE 6c

4039037 104804

FIGURE 7

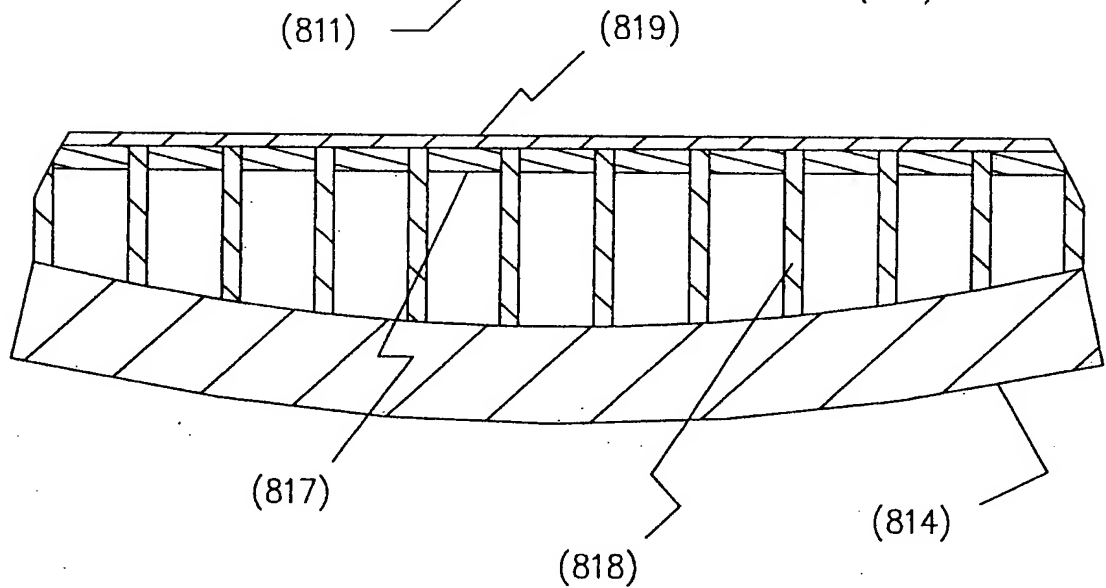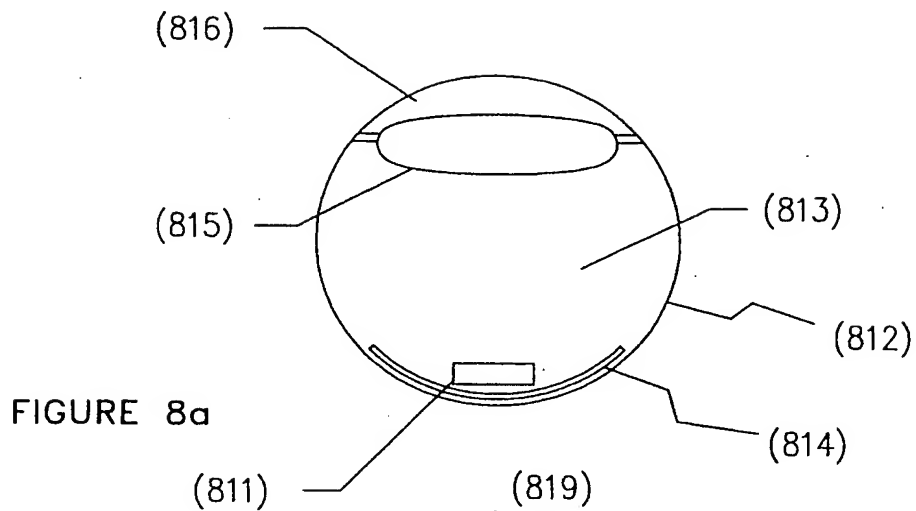

EPIRETINAL ELECTRODES - RECESSED

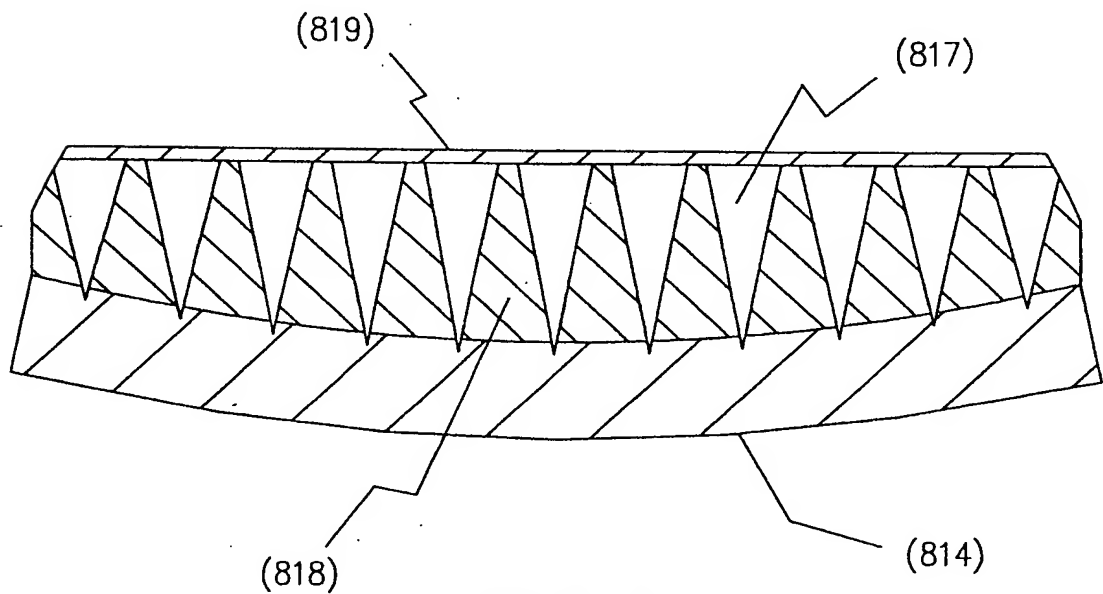

EPIRETINAL ELECTRODES - PENETRATING

403583-10-001

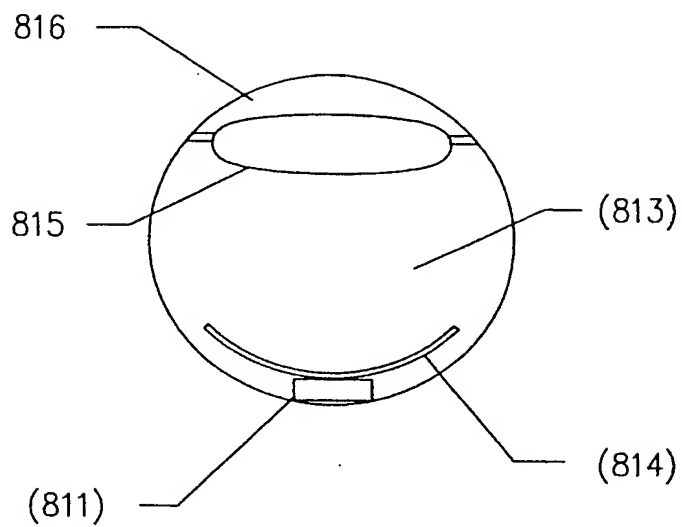


FIGURE 9a

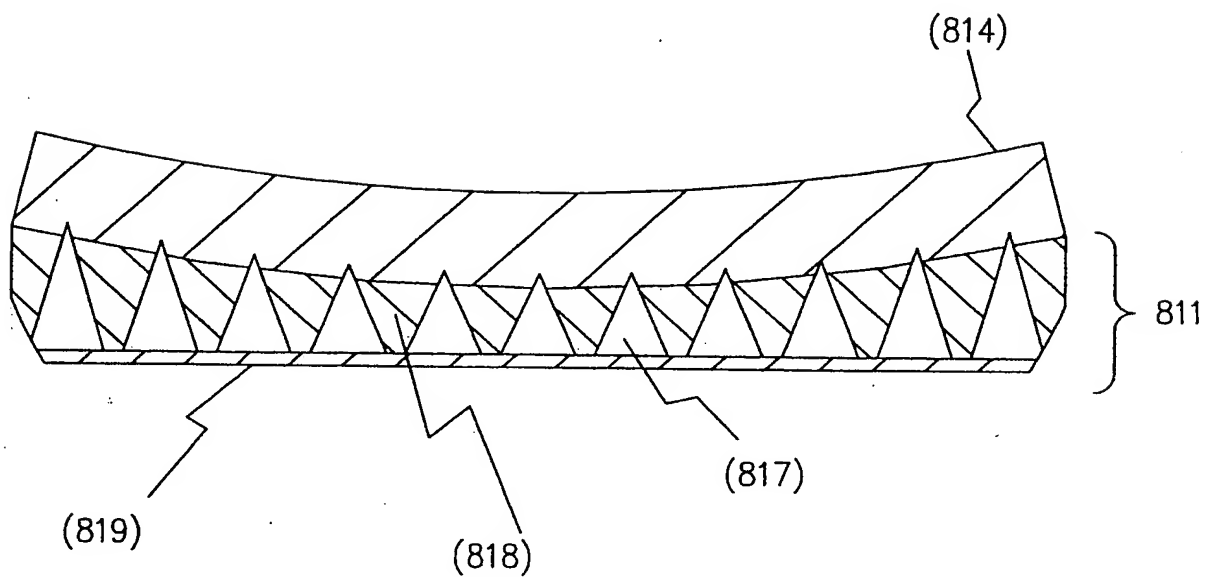


FIGURE 9b  
SUBRETINAL ELECTRODES — PENETRATING



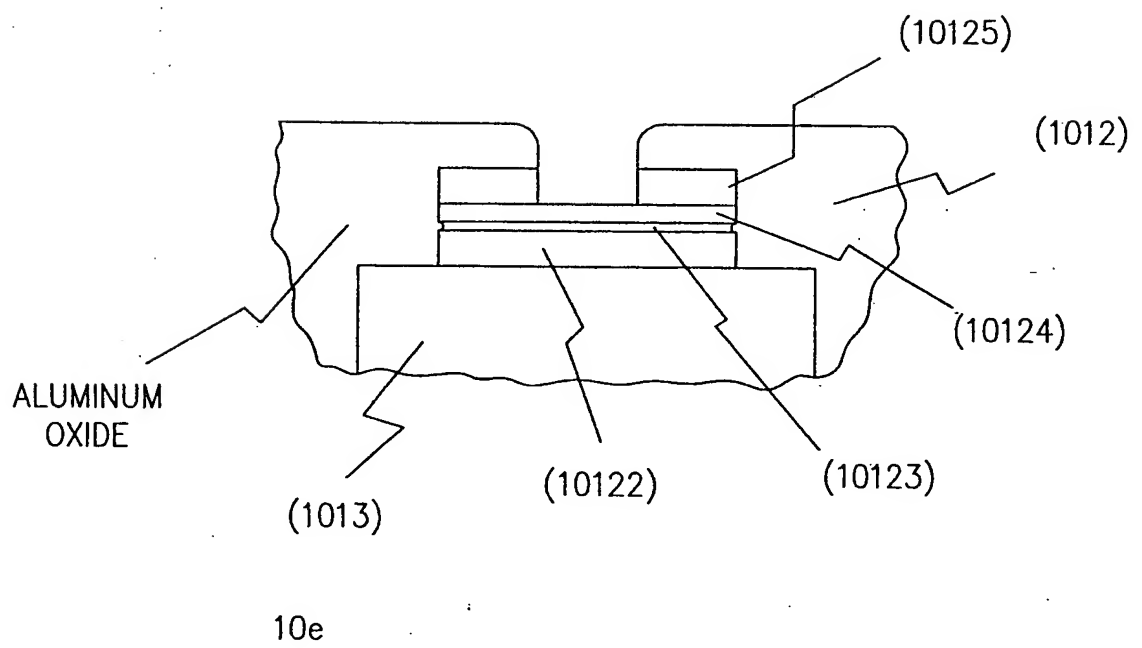
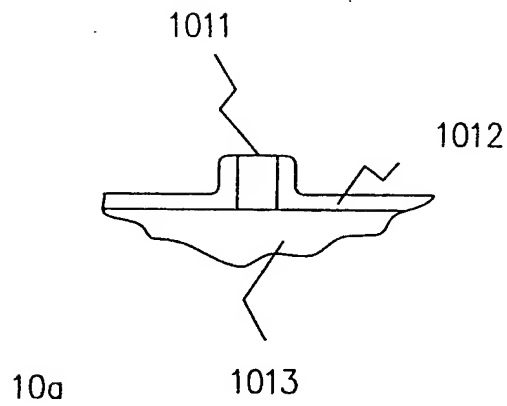
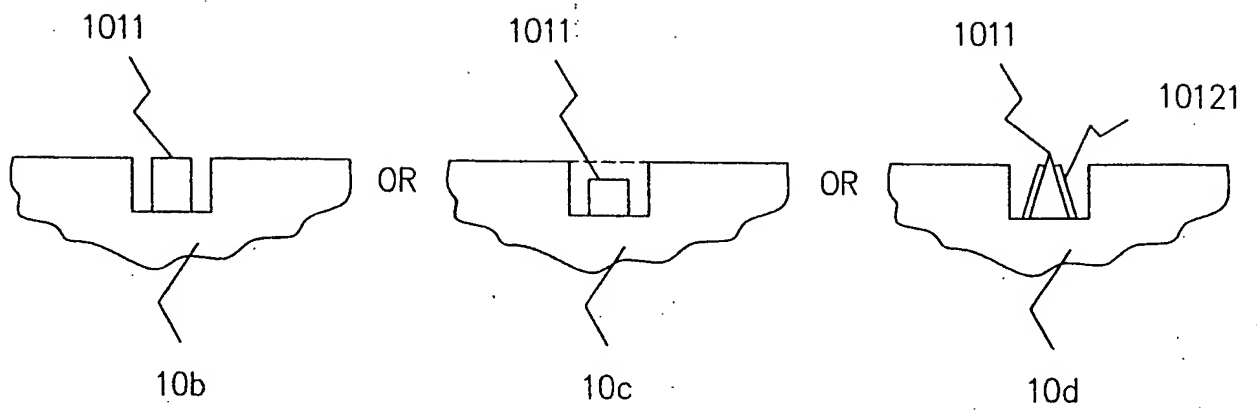


FIGURE 10

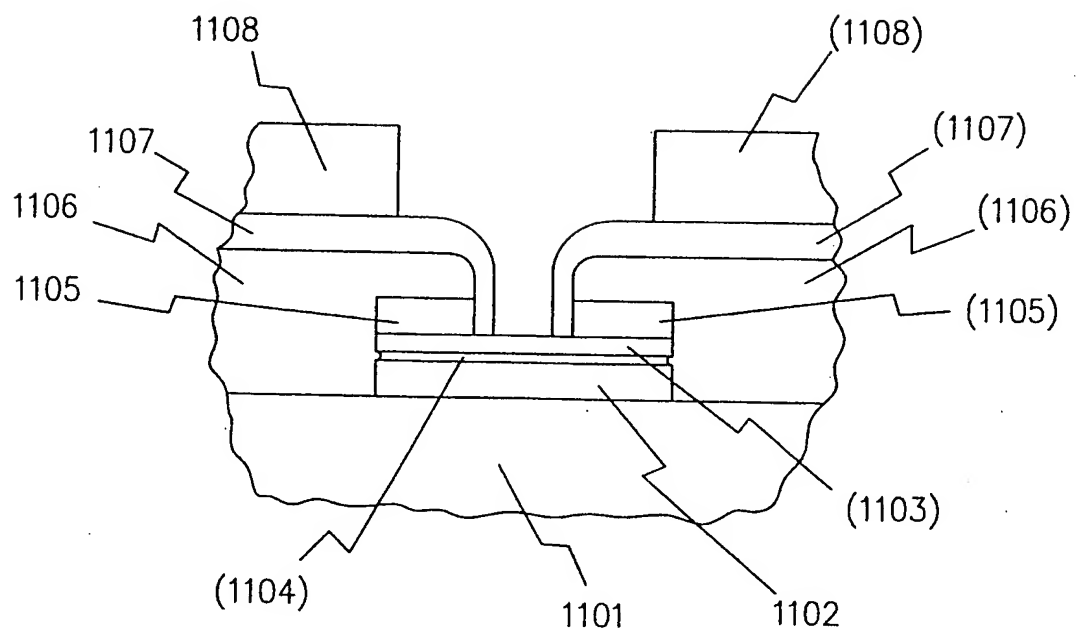


FIGURE 11a  
ELECTRODES

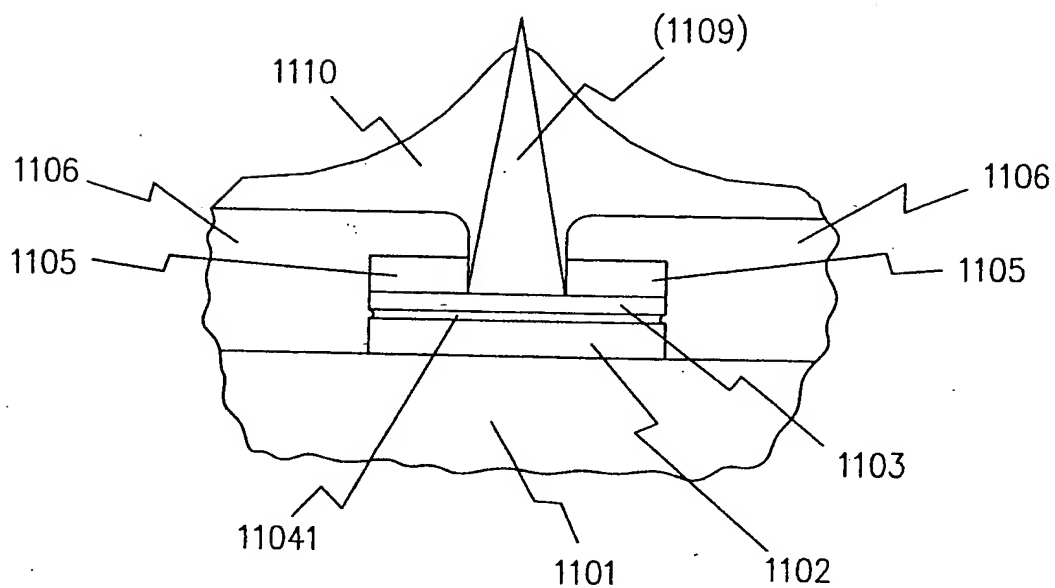


FIGURE 11b  
ELECTRODES

FIGURE 11

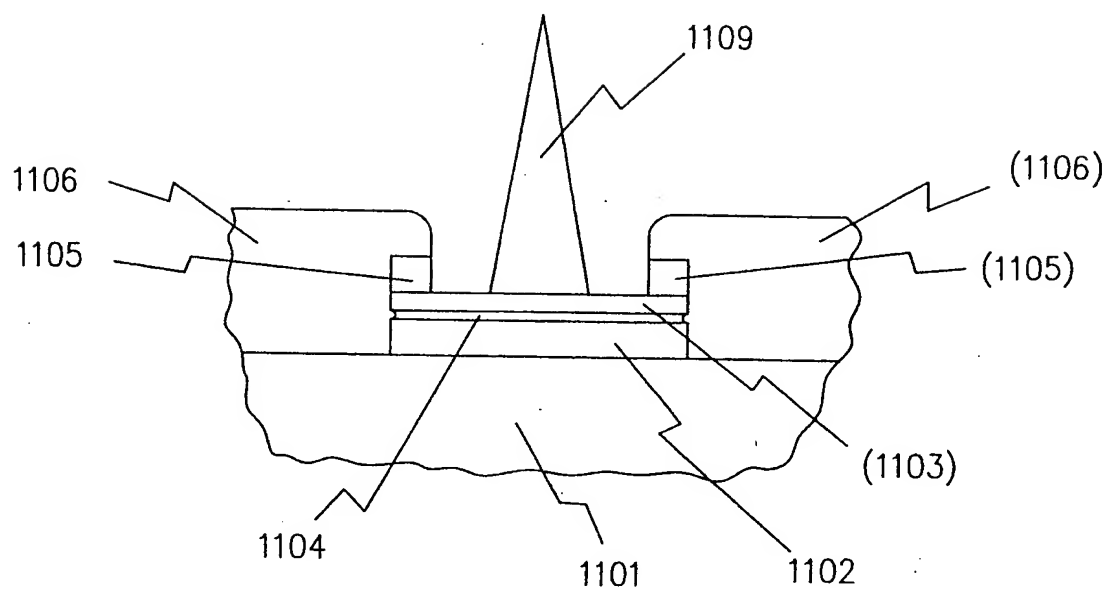


FIGURE 11c

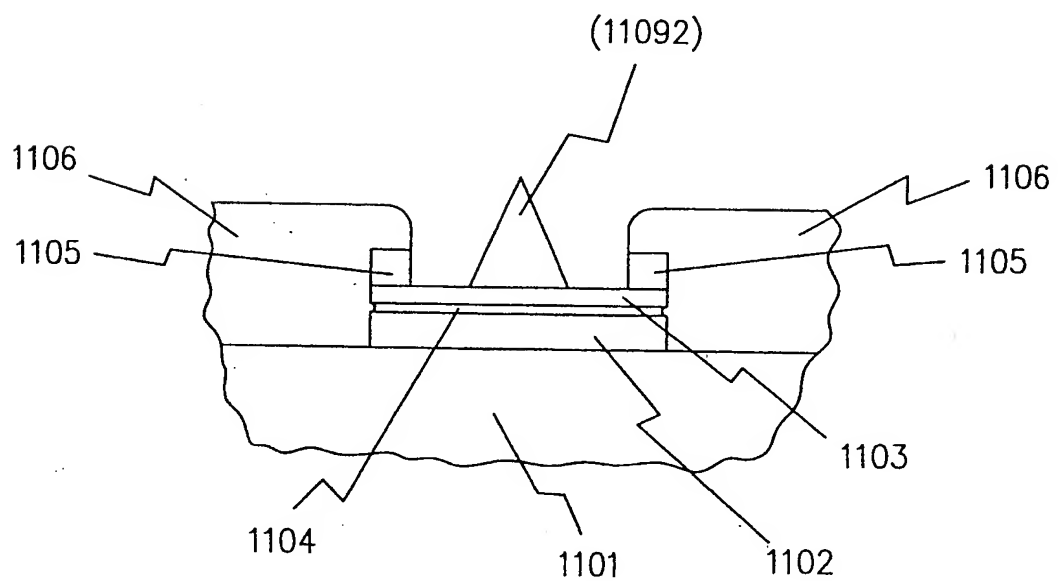


FIGURE 11d

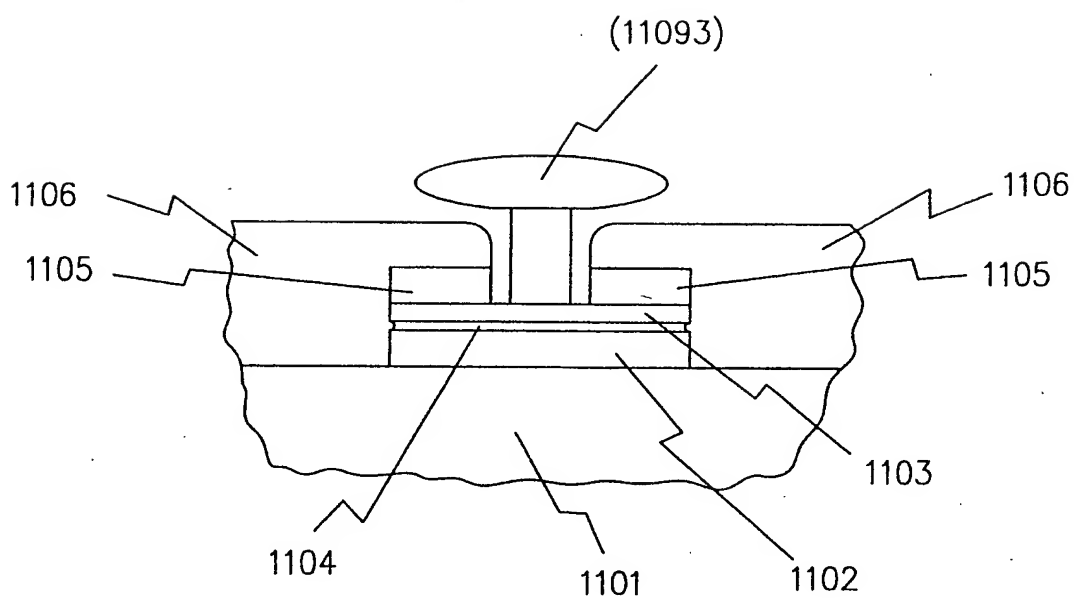


FIGURE 11e

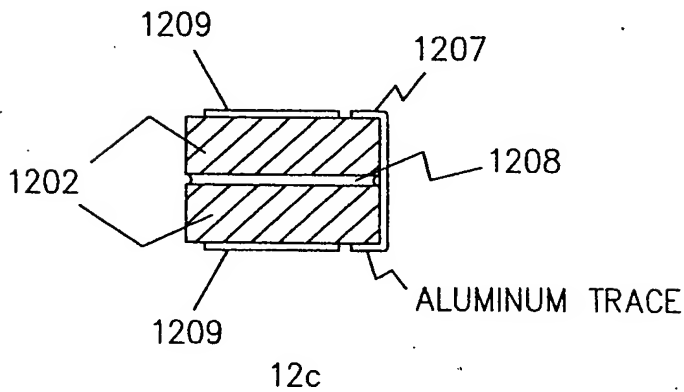
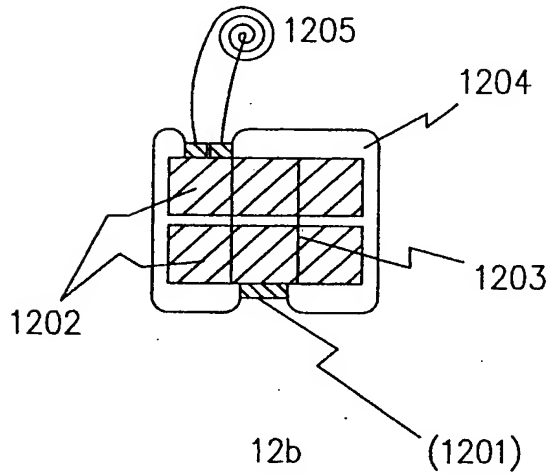
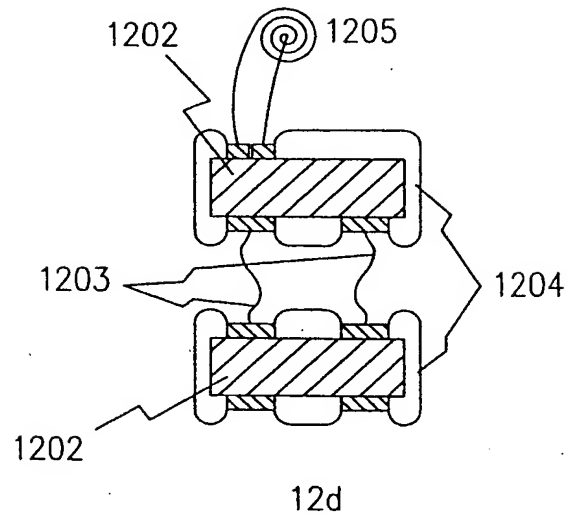
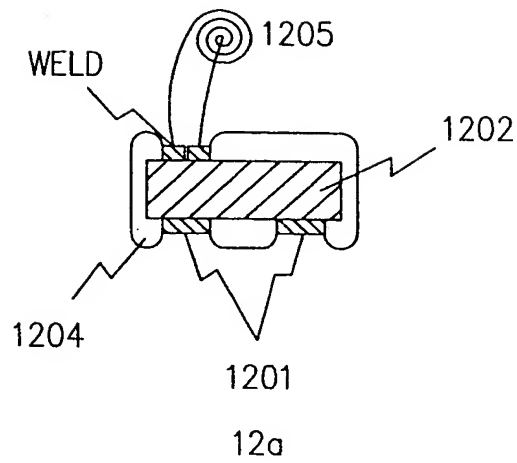


FIGURE 12  
COIL AND WIRE ATTACHMENT TO SUBSTRATES AT ELECTRODE

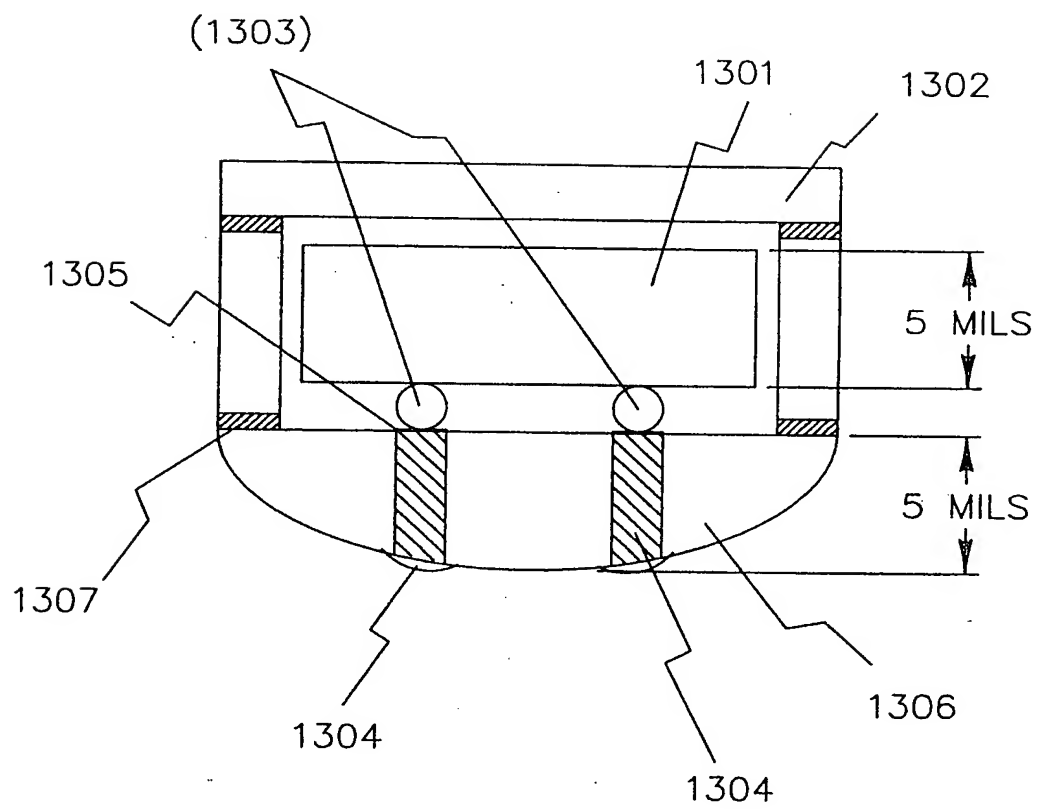


FIGURE 13  
HERMETIC SEALING

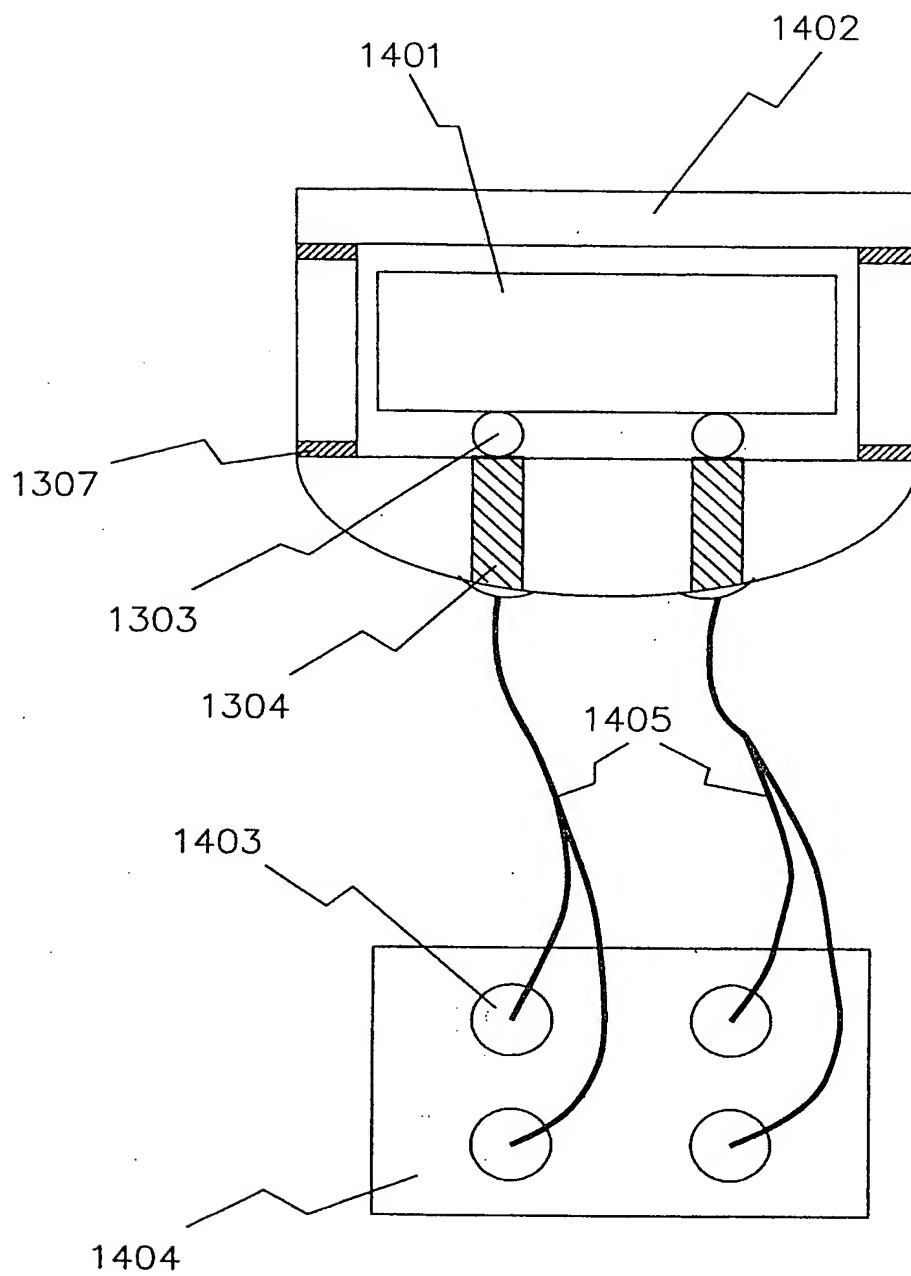


FIGURE 14

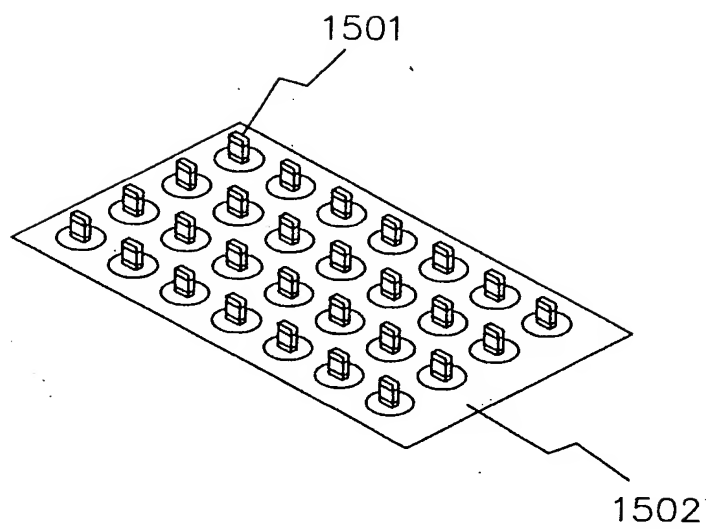


FIGURE 15



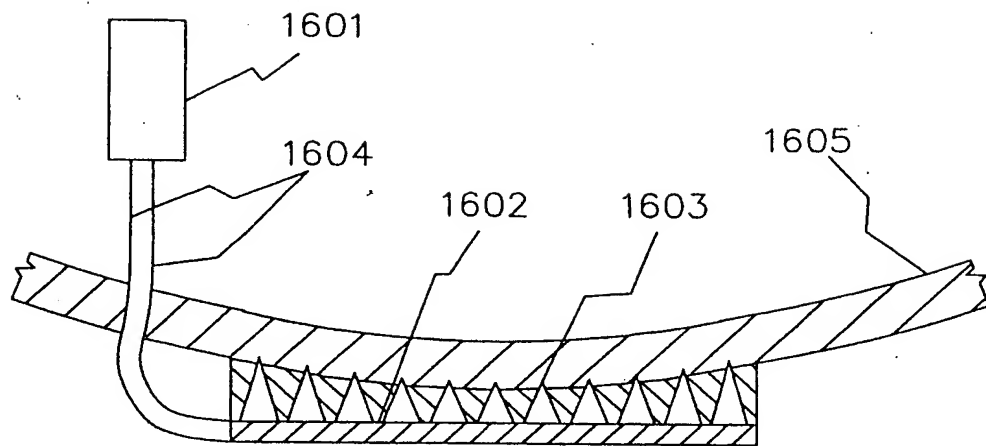


FIGURE 16a

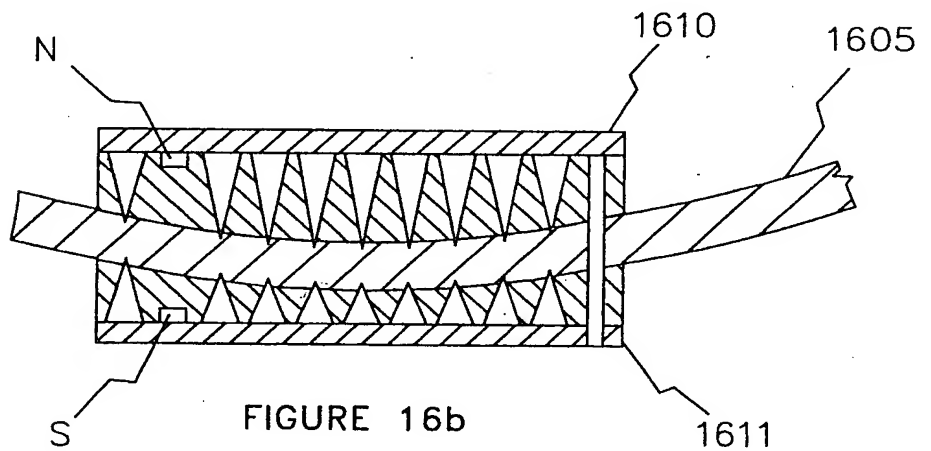


FIGURE 16b

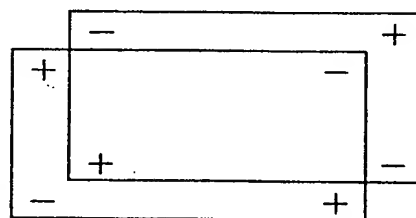


FIGURE 16c

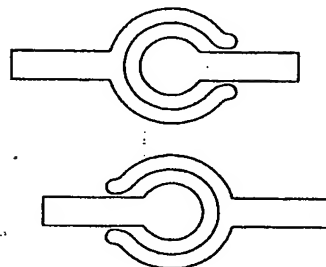


FIGURE 16d

PC PROGRAMMER

MAIN SCREEN


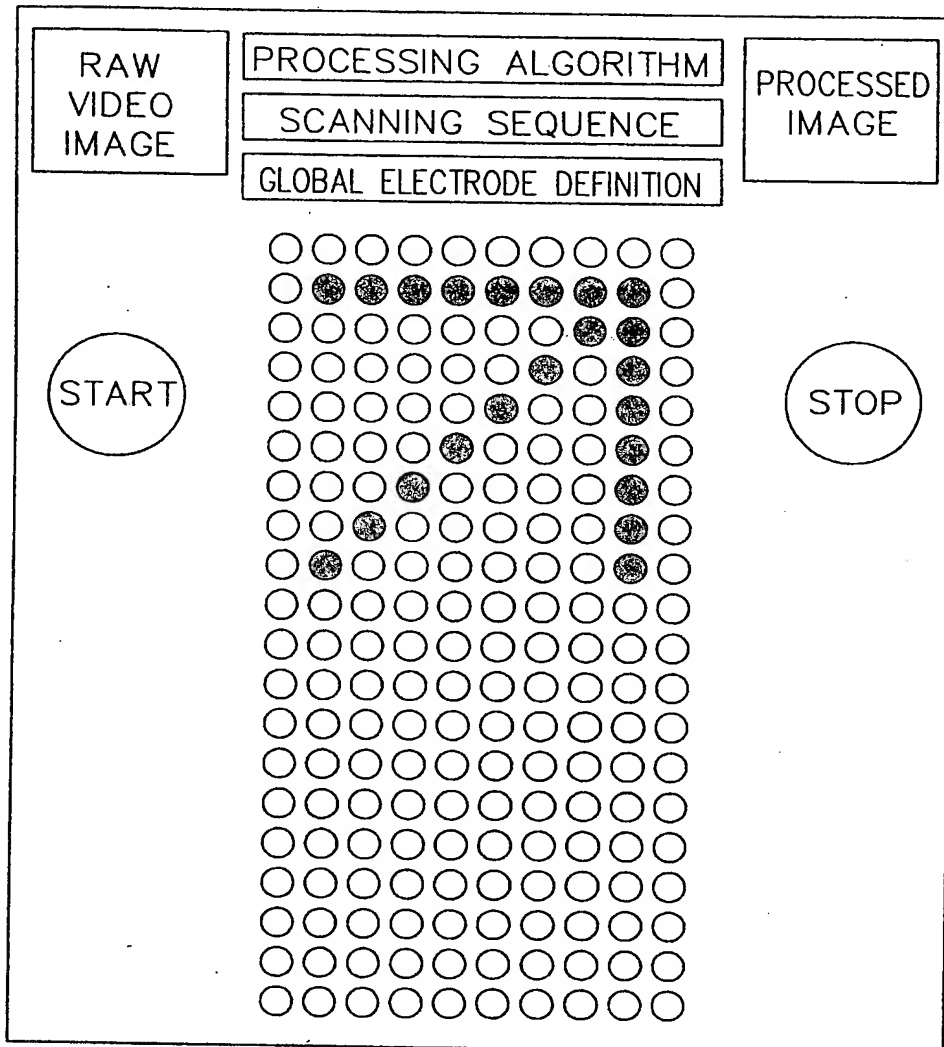


FIGURE 17a

# PROCESSING ALGORITHM


## PIXEL SELECTION

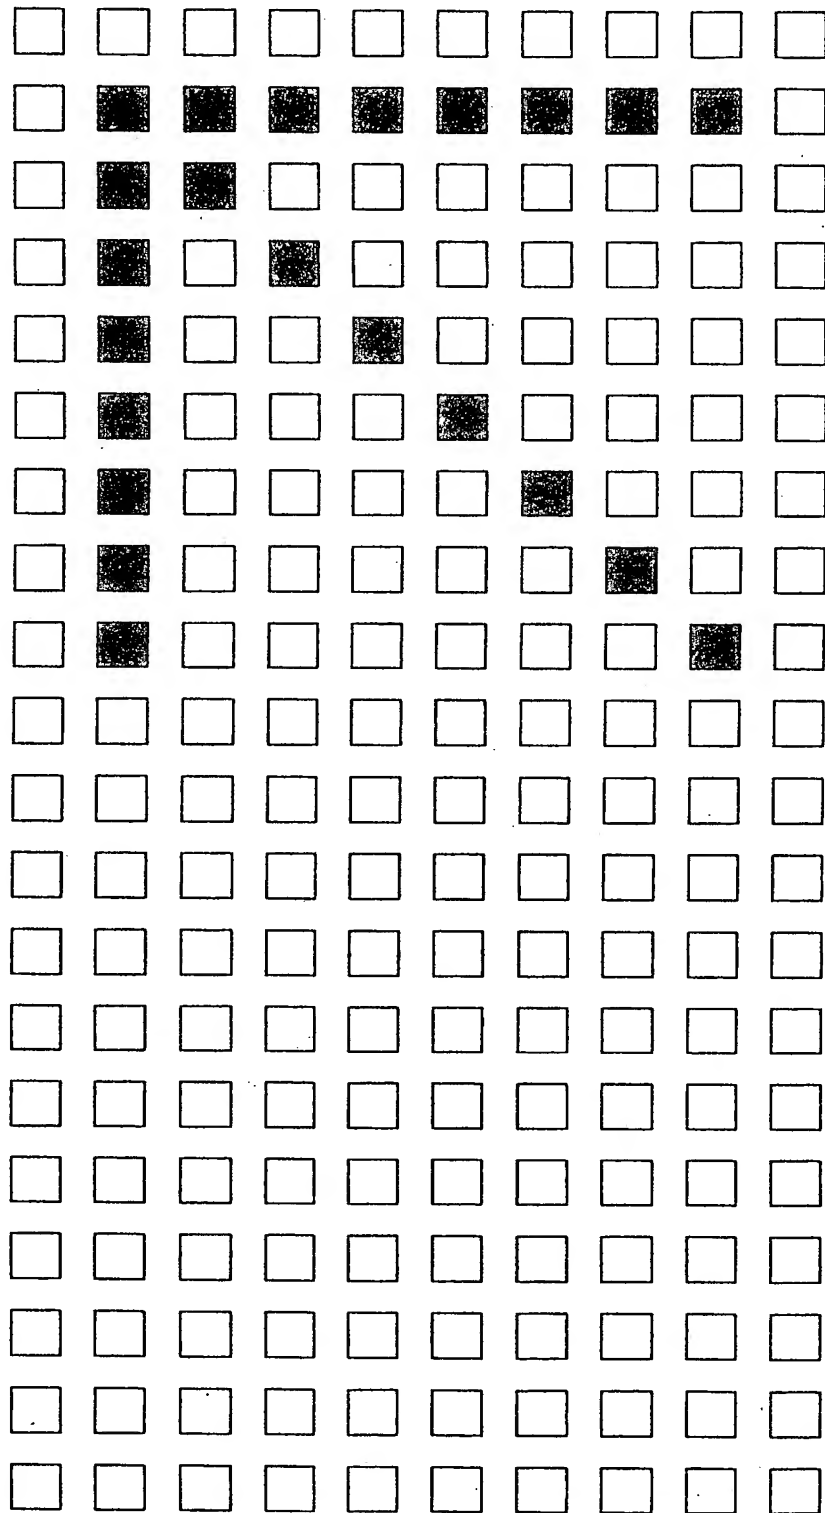

AVERAGE 8 SURROUNDING PIXELS

FIGURA 17b

# SCANNING SEQUENCE

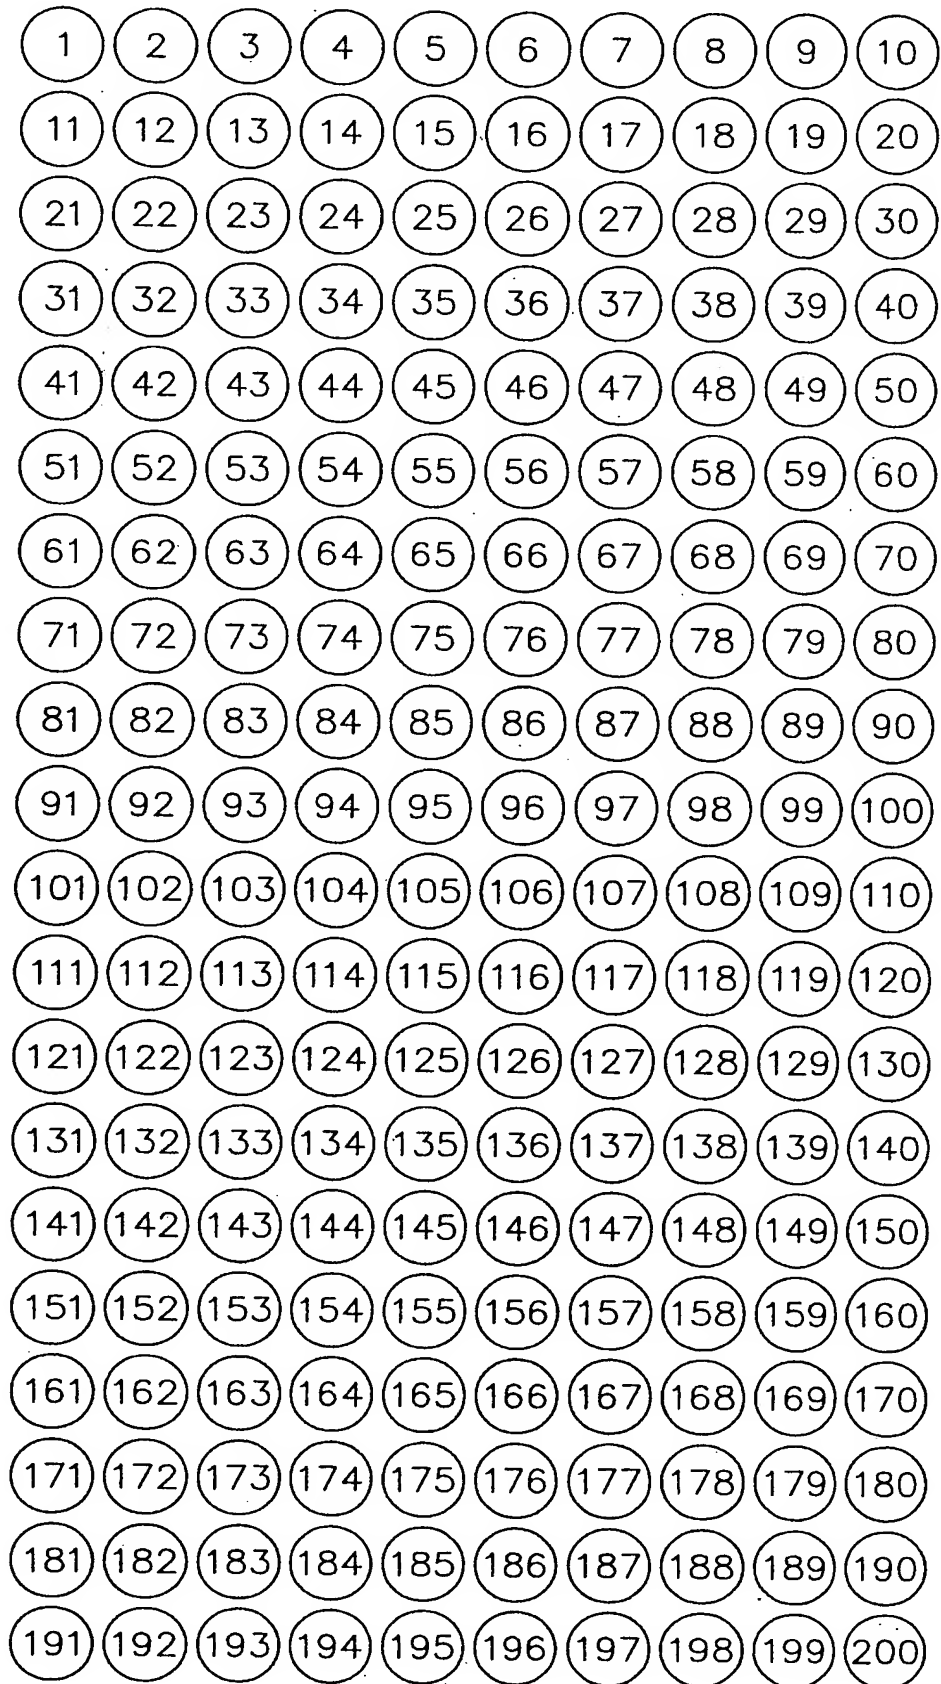

PREDEFINED SEQUENCE A

FIGURE 17c

# ELECTRODE PARAMETERS

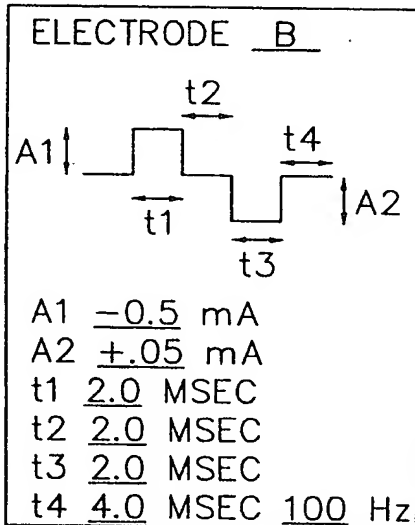


FIGURE 17d

# GLOBAL ELECTRODE CONFIGURATION

☐ MONOPOLAR  
☐ BIPOLAR  
☐ MULTIPOLAR

FIGURE 17e

## BIPOLAR

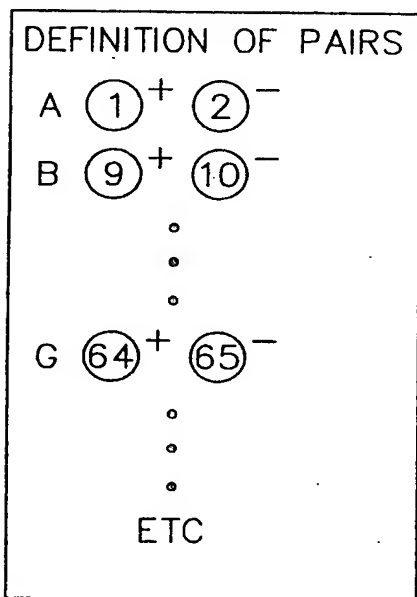


FIGURE 17f

## MULTIPOLAR

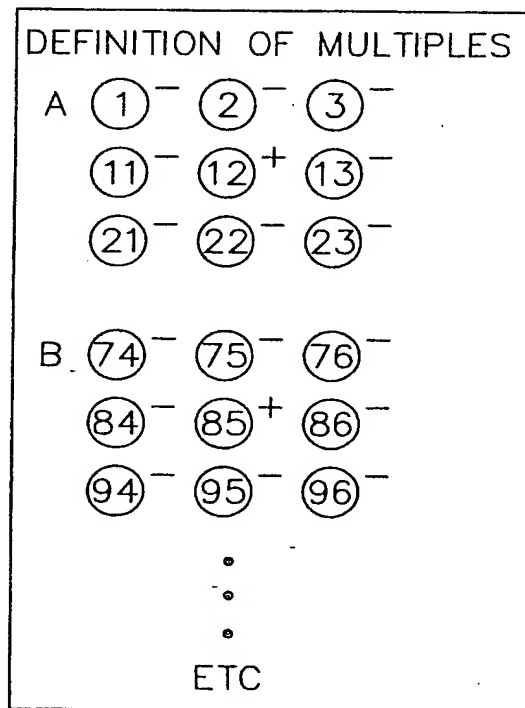


FIGURE 17g

# PALM-SIZED TEST UNIT

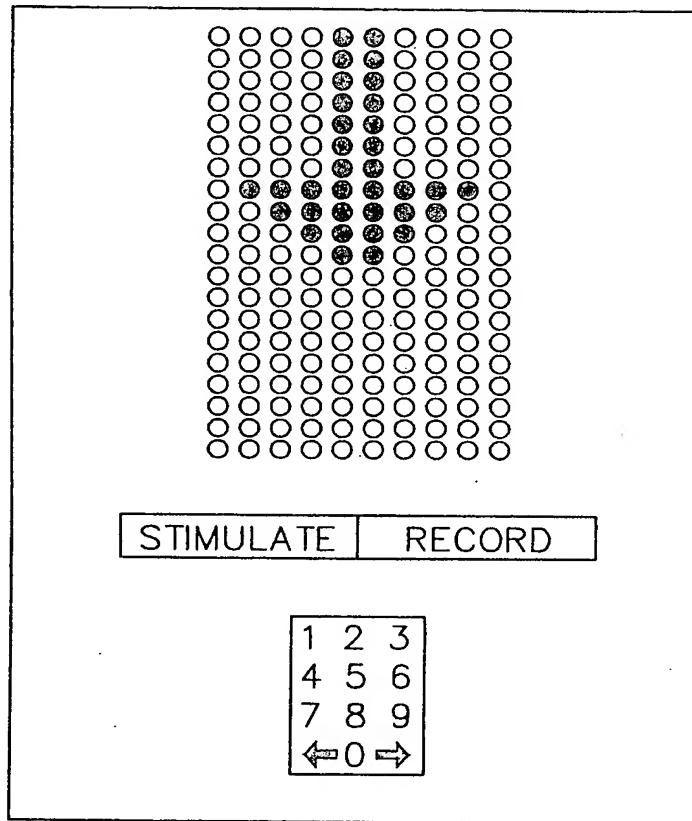


FIGURE 18a

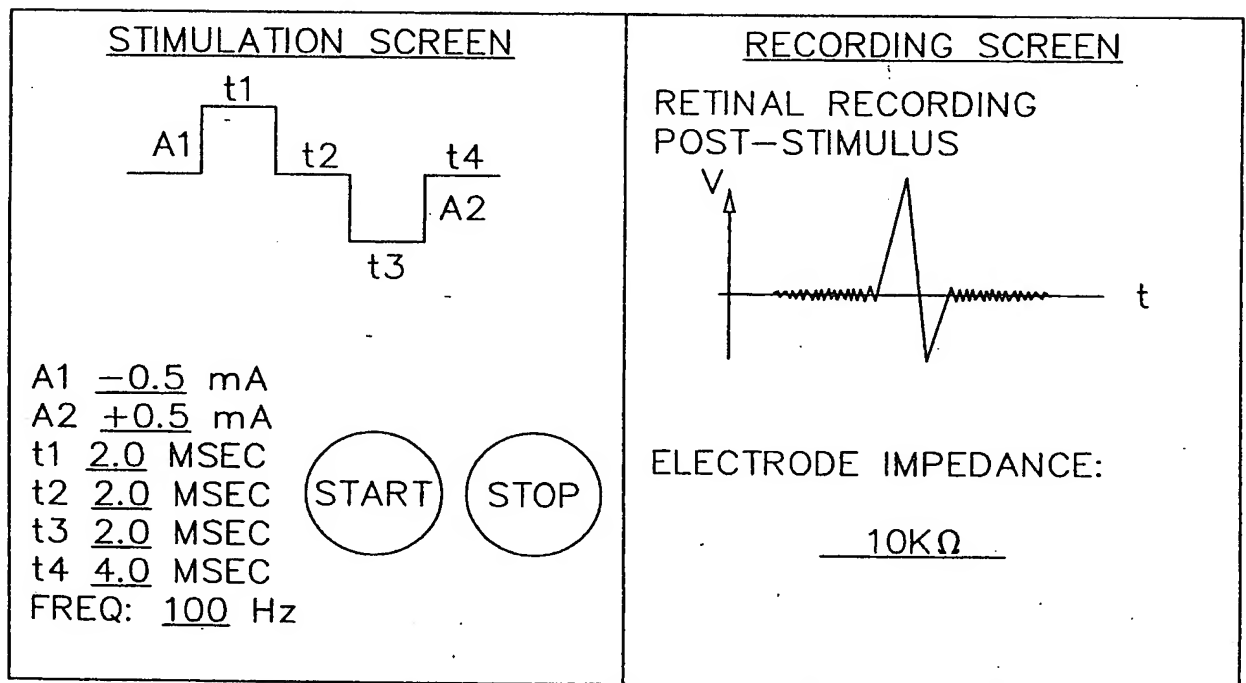


FIGURE 18b

FIGURE 18c

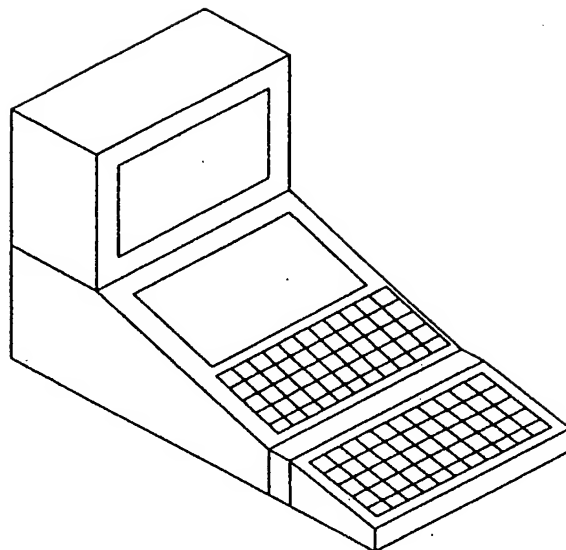


FIGURE 19a

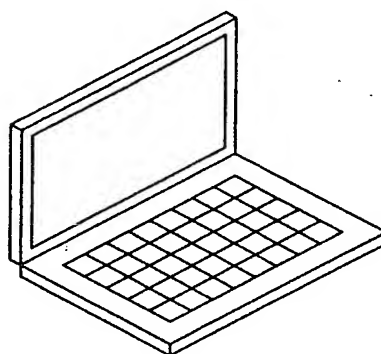


FIGURE 19b

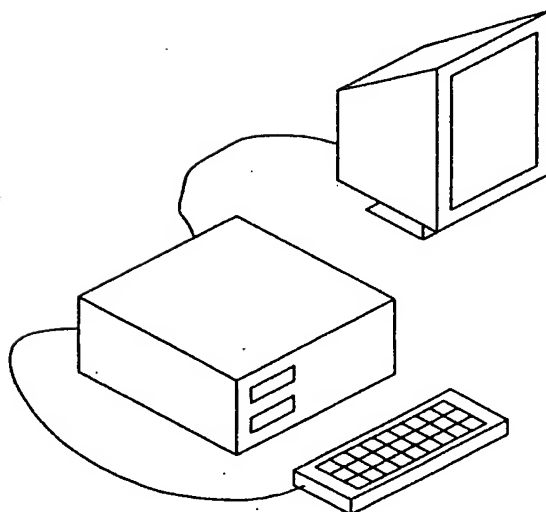


FIGURE 19c

PATIENT CONTROLLER

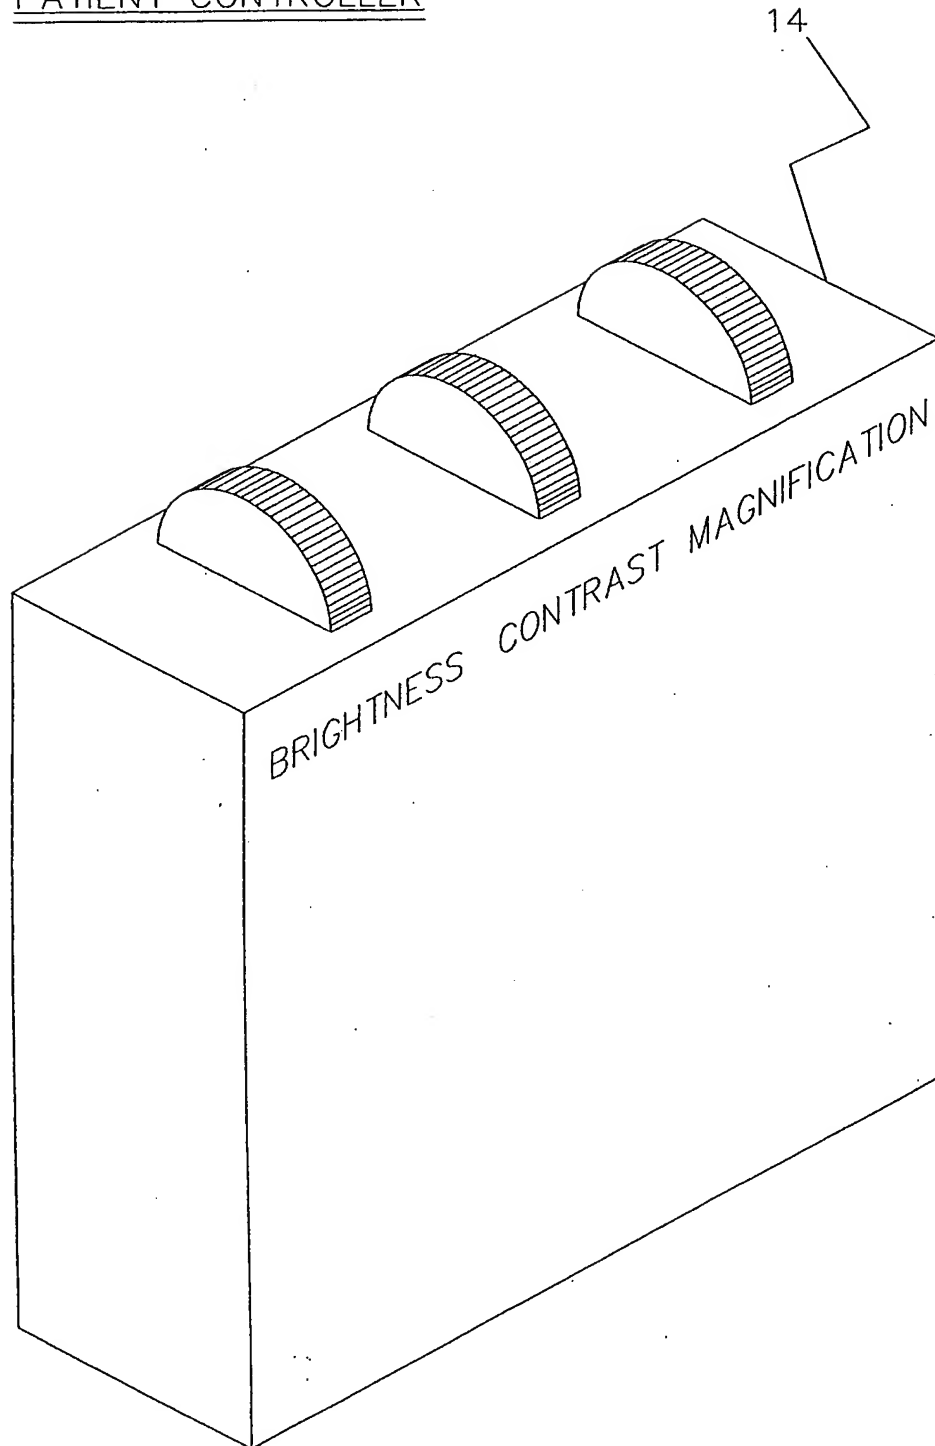


FIGURE 20